

$P_{ET}CO_2$ measured by a new lightweight mainstream capnometer with very low dead space volume offers accurate and reliable noninvasive estimation of $PaCO_2$

Daijiro Takahashi
Takehiko Hiroma
Tomohiko Nakamura

Division of Neonatology, Nagano
Children's Hospital, Nagano, Japan

Objective: Although capnometers are widely used in adult and pediatric intensive care units, they are not widely used in neonatal intensive care units due to issues such as the weight of sensors, dead space, and leakage from tracheal intubation tubes. These authors developed a light and low dead space airway adaptor of end-tidal carbon dioxide pressure ($P_{ET}CO_2$) and evaluated the correlations between $P_{ET}CO_2$ and partial CO_2 pressure ($PaCO_2$) in rabbits while changing tidal volume and leakage volume.

Methods: Firstly, Japanese rabbits weighing 2 kg were divided into three tidal volumes (6 mL/kg, 10 mL/kg, or 15 mL/kg), and $P_{ET}CO_2$ and $PaCO_2$ were measured. Secondly, the respiratory apparatus was set to a tidal volume/body weight ratio of 10 mL/kg, leakage rates were divided into seven groups, and $P_{ET}CO_2$ and $PaCO_2$ were measured.

Results: $P_{ET}CO_2$ and $PaCO_2$ were significantly correlated ($r^2 = 0.9099$, $P < 0.0001$) when there was no leakage in the tracheal intubation tubes. No significant differences were observed between $PaCO_2$ and $P_{ET}CO_2$ ($P_{a-ET}CO_2$) in the three tidal volume/body weight groups or for groups in which leakage rate was $<60\%$, but significant deviations in $P_{a-ET}CO_2$ were noted in groups with leakage rate 60% .

Conclusion: There was a strong correlation between $P_{ET}CO_2$ and $PaCO_2$ when tidal volume/body weight ratio was 6–15 mL/kg with leakage rate $<60\%$. Lightweight mainstream capnometer with a low amount of dead space airway adaptor might be useful in very low birth weight infants with small tidal volume.

Keywords: capnography, mainstream, neonate

Introduction

Advancements in the treatment of neonatal respiratory failure, including exogenous surfactant,^{1,2} inhaled nitric oxide,^{3,4} and a growing repertoire of assisted ventilation strategies,⁵ have decreased morbidity and mortality rates. Patient monitoring has played a critical role in the safe and effective application of these advanced therapies.

Maintaining partial carbon dioxide pressure ($PaCO_2$) within the desired range by frequent arterial sampling can increase the need for multiple transfusions in the neonatal intensive care unit,⁶ so methods for continuous noninvasive monitoring of CO_2 levels would prove extremely useful. Both hypocarbia and hypercarbia are detrimental to extremely low birth weight infants and have been implicated as causative factors in periventricular leukomalacia, intraventricular hemorrhage, and chronic lung disease.^{7–9} Critical event analyses have documented hypoxemia secondary to depressed

Correspondence: Tomohiko Nakamura
Division of Neonatology, Nagano
Children's Hospital 3100 Toyoshina,
Azumino City Nagano 399-8288, Japan
Tel +81 263 73 6700
Fax +81 263 73 5432
Email tnakamura@naganoch.gr.jp

respiratory activity as a principal risk factor for near misses and death.^{10,11}

Capnography, which displays the level and waveform of CO₂ in exhaled air, provides information on cell metabolism, blood perfusion, and alveolar ventilation¹² with noninvasive indirect methods. Use of end-tidal CO₂ pressure (P_{ET}CO₂) for monitoring and as a tool for verifying endotracheal tube position is a common practice in the operating room and in adult and pediatric intensive care units.¹² However, so far capnometers are not used widely in neonates due to issues such as the weight of sensors and water droplets within circuits, dead space, and leakage from tracheal intubation tubes.

These authors developed a new light (6 g) and low dead space (1 mL) airway adapter (YG-213T; Nihon-Kohden Corporation, Tokyo, Japan) for mainstream capnography (Cap-ONE TG-970P; Nihon-Kohden). The objective of this study was to evaluate the correlations between P_{ET}CO₂ and PaCO₂ in rabbits while changing tidal volume (TV) and leakage volume with this device.

Material and methods

Ten adult Japanese rabbits weighing 2 kg were anesthetized by intramuscular injection of ketamine at 10 mg/kg and xylazine at 5 mg/kg, and a 24 G catheter (JELCO, Smiths Medical Italia Srl, Mirano, Italy) was placed in the ear vein for continuous intravenous infusion of anesthetic agents. Rabbits were placed in a supine position throughout the experiment. After tracheotomy, an endotracheal tube (internal diameter, 2.5 mm; Mallinkrodt, Inc, St Louis, MO) was inserted. A 24 G catheter was placed in the internal carotid artery to allow collection of samples for blood gas analysis and to monitor arterial blood pressure and heart rate using biomedical research system (LEG-1000; Nihon-Kohden). Anesthesia was provided by continuous intravenous infusion of ketamine (5 mg/kg/hour) and paralysis was maintained by continuous administration of pancuronium (0.1 mg/kg/hour). Animals were administered a mixture of 0.45% sterile saline and 10% glucose solution at 3 mL/kg/hour during the experiment. Body temperature was continuously monitored and maintained at 38.5°C–39.5°C using a heating pad.

Rabbits were ventilated mechanically with a time-cycled pressure-limited ventilator (Humming II; Metran Co, Ltd, Saitama, Japan) adjusted to: fraction of inhaled oxygen at 0.6; inspiratory time at 0.6 seconds; and positive end-expiratory pressure at 5 cmH₂O. Peak inspiratory pressure was settled at the TV maintained at TV/body weight (BW) ratios of 6 mL/kg, 7 mL/kg, 10 mL/kg, and 15 mL/kg, as measured by pneumotachography (ARFEL-VR; Aivision Corporation,

Tokyo, Japan). Respiratory rate was adjusted to a level at which normocapnia was maintained (41.6 ± 3.8 mmHg). In the investigation of the effects on TV/BW, TV/BW was divided into three groups (6 mL/kg, 10 mL/kg, and 15 mL/kg), and P_{ET}CO₂ and PaCO₂ was measured.

P_{ET}CO₂ was monitored in intubated rabbits by mainstream capnography (Cap-One TG-970P; Nihon-Kohden). Mainstream P_{ET}CO₂ was measured via a capnograph connected to the proximal end of the endotracheal tube. Before each blood sampling, an adequate reading of P_{ET}CO₂ and a reliable waveform on the mainstream capnograph (continuous steady waveform of expired CO₂ throughout the ventilatory cycle) was taken. Data was continuously recorded on a laptop computer using the software programmed by LabVIEW (National Instruments Corporation, Austin, TX) for each rabbit. PaCO₂ was measured from samples withdrawn intermittently from intraarterial lines indwelling in the internal carotid artery (ABL700; Radiometer Medical ApS, Bronshoj, Denmark). The amount of leakage was adjusted by fixation of the tracheal intubation tubes. The leakage ratio was calculated using the following equation:

$$\text{Leakage ratio} = (\text{inspiratory TV} - \text{expiratory TV}) / \text{inspiratory TV} \times 100$$

The end-tidal volume was measured by mainstream capnography (CO2SMO 8100, Fukuda Denshi, Tokyo, Japan) and also leakage rate was calculated with CO2SMO 8100. The respiratory apparatus was set to a TV/BW ratio of 10 mL/kg, then leakage rates were divided into seven groups (0%–10%, 10%–30%, 30%–50%, 50%–60%, 60%–70%, 70%–80%, and 80%–100%), and P_{ET}CO₂ and PaCO₂ were measured.

PaCO₂ was measured with the additional dead space caused by attachment of a CO₂ sensor and additional dead space in the setting of TV/BW ratios of 6 mL/kg, 7 mL/kg, and 10 mL/kg.

Statistical analyses were conducted using SPSS Statistics version 17.0 software (SPSS, Inc, Chicago, IL). To determine whether P_{ET}CO₂ values were representative of PaCO₂, the relationship between P_{ET}CO₂ and PaCO₂ was analyzed by simple linear regression. Bland–Altman plots, representing a visual assessment of agreement between two methods of measurement, were created to assess the measurement of P_{ET}CO₂. Bland–Altman plots demonstrate “good agreement” not only when differences between methods are consistent across all measurements but also when the differences are small. In a situation in which difference between the two measurements is expected to change based on a third

variable, Bland–Altman plots lose importance. The precision of $P_{ET}CO_2$ measurements and agreement between $P_{ET}CO_2$ and $PaCO_2$ values were assessed by bias ($PaCO_2 - P_{ET}CO_2$), standard deviation, and 95% confidence interval (CI) for the bias. One-factor analysis of variance and the Mann–Whitney U test were used to compare differences between subgroups of TV/BW and leakage ratio. Values of $P < 0.05$ were considered significant. The present study was conducted with the approval of the Institutional Animal Care and Use Committee of Nagano Children's Hospital, Nagano, Japan.

Results

A total of 43 measurements of $P_{ET}CO_2$ and $PaCO_2$ were analyzed. Under conditions of no leakages in the tracheal intubation tubes, $P_{ET}CO_2$ and $PaCO_2$ were significantly correlated ($r^2 = 0.9099$, $P < 0.0001$; Figure 1) and the Bland–Altman plot test showed a mean difference (bias) for $P_{ET}CO_2$ of -0.876 mmHg (Figure 2). The 95% CI for this bias was -1.80 – 0.04 mmHg. The 95% CI of limits of agreement was -6.74 – 4.99 mmHg.

In the comparison of differences between $PaCO_2$ and $P_{ET}CO_2$, when setting the TV/BW to 6 mL/kg, 10 mL/kg or 15 mL/kg, no significant differences were observed between the three groups (Figure 3).

Figure 4 shows the effects of additional dead space on $PaCO_2$ under TV conditions of 12 mL, 14 mL, or 20 mL. Under TV conditions of 12 mL and 14 mL (6 mL/kg and 7 mL/kg, respectively), $PaCO_2$ was significantly increased by a dead space increase of only 1 mL, but under TV conditions of 20 mL (10 mL/kg), a dead space increase of 1 mL did not significantly increase $PaCO_2$. $PaCO_2$ thus seemed to be increased by dead space increases representing 7% of TV.

Figure 5 shows the effects of leakage rate on $PaCO_2/P_{ET}CO_2$ at a TV/BW of 10 mL/kg. For all leakage rates $<60\%$, no significant differences were seen between $PaCO_2$ and $P_{ET}CO_2$

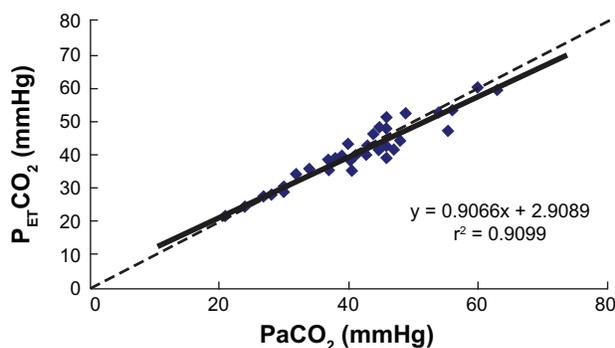


Figure 1 End-tidal carbon dioxide pressure ($P_{ET}CO_2$) and partial CO_2 pressure ($PaCO_2$) were significantly correlated ($r^2 = 0.9099$, $P < 0.0001$).
Note: Dotted line is the line of identity.

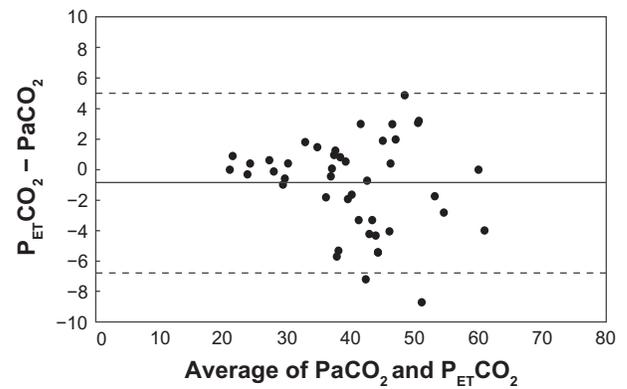


Figure 2 In the Bland–Altman plot test, the mean difference (bias) and standard deviation of differences for end-tidal carbon dioxide pressure ($P_{ET}CO_2$) was -0.876 ± 2.99 mmHg. The 95% confidence interval for bias was -6.74 to 4.99 mmHg.
Abbreviation: $PaCO_2$, partial CO_2 pressure.

compared to the group with a leakage rate of 0%–10%. However, groups with leakage rate 60% showed significant deviations between $PaCO_2$ and $P_{ET}CO_2$.

Regarding the expiratory plateau phase, a relatively constant PCO_2 was maintained when alveolar mixed gas was expired, as shown by the capnogram for 10 mL/kg TV/BW and leakage ratio $<60\%$ (Figure 6).

Discussion

It was found that $P_{ET}CO_2$ measured by mainstream capnography cap-ONE was an accurate and reliable noninvasive method for estimating $PaCO_2$, showing a good correlation with $PaCO_2$ ($r^2 = 0.9099$, $P < 0.0001$), and there is no bias in the measurement (95% CI: -1.80 – 0.04 mmHg).

$P_{ET}CO_2$ can be feasibly measured by mainstream or sidestream capnography. Measuring $P_{ET}CO_2$ reportedly underestimates alveolar CO_2 due to the relatively low TVs and rapid respiratory rates of newborns.^{13,14} The CO_2 waveform (capnogram) has been characterized for adult patients with normal and abnormal pulmonary function.^{15,16} In newborns,

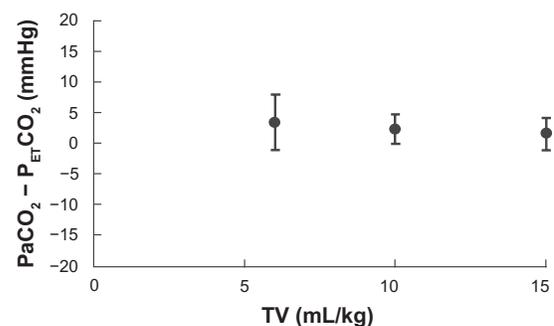


Figure 3 In the comparison of differences between end-tidal carbon dioxide pressure ($P_{ET}CO_2$) and partial CO_2 pressure ($PaCO_2$), no significant differences were observed between the three groups with tidal volume (TV)/body weight ratio of 6 mL/kg, 10 mL/kg, and 15 mL/kg.

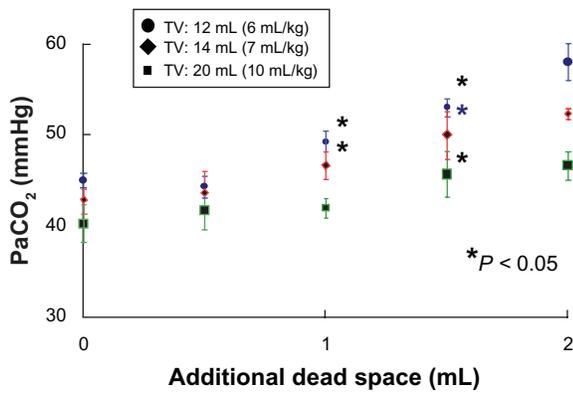


Figure 4 Effects of additional dead space on partial carbon dioxide pressure (PaCO₂) under conditions of 12 mL or 20 mL of tidal volume (TV). Under conditions of 12 mL of TV (6 mL/kg), PaCO₂ was significantly increased by a dead space increase of only 1 mL. Under conditions of 20 mL of TV (10 mL/kg), even a dead space increase of 1 mL did not significantly increase PaCO₂. PaCO₂ appears to be affected by a dead space increase of >7% of TV.

CO₂ waveform slurring (a spurious decrease in the slope of the ascending phase of the capnogram) occurs due to dilution of exhaled gas when small, rapid breath packets are measured in a relatively large sample cell.¹⁷

Condensed water and patient secretions may also impede both mainstream and sidestream technologies. Furthermore, relative inaccuracy is seen in conditions of ventilation-perfusion mismatch.^{18,19}

Transcutaneous CO₂ monitoring is a noninvasive technique for measuring CO₂ levels. However, transcutaneous CO₂ monitoring is not tolerated in very low birth weight infants because of their fragile skin, and the technique is affected by acidosis and hypoxia.^{20,21}

Mainstream capnography has been found to be more accurate,²²⁻²⁴ but the sensor position used for mainstream capnography is connected inline between the proximal



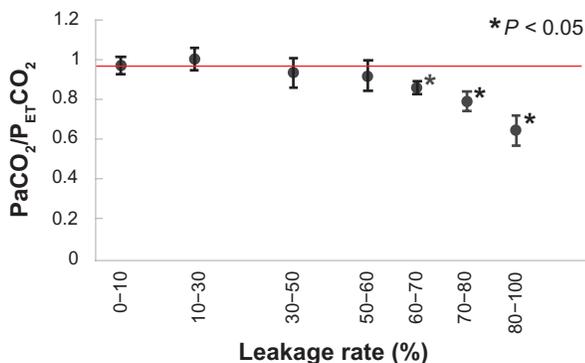


Figure 5 Effects of leakage rate on end-tidal carbon dioxide pressure (P_{ET}CO₂) and partial CO₂ pressure (PaCO₂). When leakage rate was <60%, no significant differences were seen between PaCO₂ and P_{ET}CO₂ compared to the group in which the leakage rate was 0%–10%. However, groups with leakage rate 60% showed significant deviations between PaCO₂ and P_{ET}CO₂.

✓ TV/BW 10 mL/kg, leakage rate 4%, PaCO₂ 42 mmHg

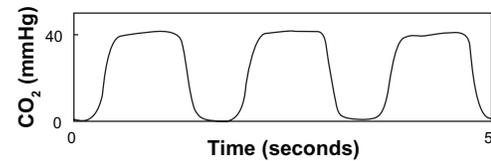

✓ TV/BW 10 mL/kg, leakage rate 62%, PaCO₂ 39 mmHg

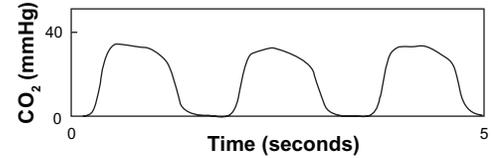

✓ TV/BW 10 mL/kg, leakage rate 92%, PaCO₂ 39 mmHg

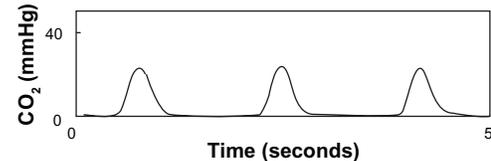


Figure 6 Regarding the expiratory plateau phase, when alveolar mixed gas was expired, a relatively constant partial CO₂ pressure (PaCO₂) was maintained, as shown by the capnogram for the >6 mL/kg tidal volume/body weight (TV/BW) group.

endotracheal tube and ventilator circuit. As a result, dead space is increased, the sensor competes for TV, and sensor weight may kink the endotracheal tube. When a flow sensor is connected to the endotracheal tube, use of mainstream capnography is even more cumbersome.²⁵ Given these limitations, most neonatal intensive care units do not routinely perform capnography to assess and manage ventilatory status. These problems might be reduced in measurement of P_{ET}CO₂ if the sensor is lightweight and the dead space is small.

In the comparison of differences between PaCO₂ and P_{ET}CO₂, when setting the TV/BW to 6 mL/kg, 10 mL/kg, or 15 mL/kg, no significant differences were observed between the three groups even at the 6 mL/kg setting. Conversely, Sakamoto et al reported a lower correlation between PaCO₂ and P_{ET}CO₂ with ≤6 mL/kg compared to >6 mL/kg in porcine neonates.²⁶ They measured P_{ET}CO₂ by sidestream capnography, so P_{ET}CO₂ might have been underestimated.

Figure 4 shows the effects of additional dead space on PaCO₂. Under conditions of 6 mL/kg of TV, PaCO₂ was significantly increased by a dead space increase of only 1 mL, representing >7% of TV. Figueras et al²⁷ reported that the introduction of the pneumotachometer, which has a dead space of 1.6 mL for 10 minutes, led to a transcutaneous PCO₂ increase of 5.40 ± 2.66 mmHg, from 39.76 ± 8.69 mmHg to 45.17 ± 9.22 mmHg (P = 0.0000) in newborn infants. However, they did not measure PaCO₂ directly, nor they did change the amount of dead space when measuring transcutaneous PCO₂.

With respect to lung injury, too high volumes/pressures and/or too low positive end expiratory pressure promotes degradation of the lungs, so-called ventilator-induced lung injury, and is associated with high mortality.²⁸ Such injuries are known to result in local alterations in lung compliance and pulmonary edema secondary to capillary leakage and are important contributing factors to the pathogenesis of chronic lung disease in neonates.^{29,30}

To the best of the authors' knowledge, no studies have described the effects of endotracheal tube leakage on $P_{ET}CO_2$. Leakage is more of a problem in children than in adults because of the use of uncuffed endotracheal tubes. Capnography offers direct monitoring of the inhaled and exhaled concentrations or partial pressure of CO_2 . The amount of endotracheal tube leakage around an uncuffed endotracheal tube is thus larger, and significant differences between $PaCO_2$ and $P_{ET}CO_2$ might arise.

No significant differences were found between $PaCO_2$ and $P_{ET}CO_2$ when the leakage rate was <60%, similar to the group in which leakage rate was 0%–10%. However, in groups with a leakage rate 60%, significant deviations were seen between $PaCO_2$ and $P_{ET}CO_2$.

Also, regarding the expiratory plateau phase, a relatively constant PCO_2 was maintained, as shown by the capnogram for 10 mL/kg TV/BW and leakage ratio <60% (Figure 6).

This analysis of rabbits weighing 2 kg revealed good correlation and agreement between $PaCO_2$ and $P_{ET}CO_2$. However, only deep anesthetized rabbits weighing 2 kg were used. In addition, $P_{ET}CO_2$ was measured in rabbits using the setting of limited mechanical ventilation. Further studies using different conditions are warranted to further elucidate this area.

Conclusion

A strong correlation was obtained and there was no bias between $P_{ET}CO_2$ and $PaCO_2$ when TV/BW was 6–15 mL/kg and the leakage rate was <60%. Lightweight and low amounts of dead space capnometer may be used in very low birth weight infants with small TV.

Disclosure

The authors report no conflicts of interest in this work.

References

- Lee K, Khoshnood B, Wall SN, Chang Y, Hsieh HL, Singh JK. Trend in mortality from respiratory distress syndrome in the United States, 1970–1995. *J Pediatr*. 1999;134(4):434–440.
- Rodriguez RJ, Martin RJ. Exogenous surfactant therapy in newborns. *Respir Care Clin N Am*. 1999;5(4):595–616.
- Wessel DL, Adatia I, Van Marter LJ, et al. Improved oxygenation in a randomized trial of inhaled nitric oxide for persistent pulmonary hypertension of the newborn. *Pediatrics*. 1997;100(5):E7.
- Cornfield DN, Maynard RC, deRegnier RA, Guiang SF 3rd, Barbato JE, Milla CE. Randomized, controlled trial of low-dose inhaled nitric oxide in the treatment of term and near-term infants with respiratory failure and pulmonary hypertension. *Pediatrics*. 1999;104(5 Pt 1):1089–1094.
- Plavka R, Kopecky P, Sebron V, Svihovec P, Zlatohlavkova B, Janus V. A prospective randomized comparison of conventional mechanical ventilation and very early high frequency oscillatory ventilation in extremely premature newborns with respiratory distress syndrome. *Intensive Care Med*. 1999;25(1):68–75.
- Madsen LP, Rasmussen MK, Bjerregaard LL, Nohr SB, Ebbesen F. Impact of blood sampling in very preterm infants. *Scand J Clin Lab Invest*. 2000;60(2):125–132.
- Giannakopoulou C, Korakaki E, Manoura A, et al. Significance of hypocarbia in the development of periventricular leukomalacia in preterm infants. *Pediatr Int*. 2004;46(3):268–273.
- Erickson SJ, Grauaug A, Gurrin L, Swaminathan M. Hypocarbia in the ventilated preterm infant and its effect on intraventricular haemorrhage and bronchopulmonary dysplasia. *J Paediatr Child Health*. 2002;38(6):560–562.
- Wallin LA, Rosenfeld CR, Luptook AR, et al. Neonatal intracranial hemorrhage: II. Risk factor analysis in an inborn population. *Early Hum Dev*. 1990;23(2):129–137.
- Wiswell TE, Graziani LJ, Kornhauser MS, et al. Effects of hypocarbia on the development of cystic periventricular leukomalacia in premature infants treated with high-frequency jet ventilation. *Pediatrics*. 1996;98(5):918–924.
- Strauss RG. Transfusion therapy in neonates. *Am J Dis Child*. 1991;145(8):904–911.
- Bhende MS. End-tidal carbon dioxide monitoring in pediatrics – clinical applications. *J Postgrad Med*. 2001;47(3):215–218.
- Kirpalani H, Kechagias S, Lerman J. Technical and clinical aspects of capnography in neonates. *J Med Eng Technol*. 1991;15(4–5):154–161.
- Badgwell JM, Heavner JE, May WS, Goldthorn JF, Lerman J. End-tidal PCO_2 monitoring in infants and children ventilated with either a partial rebreathing or a non-rebreathing circuit. *Anesthesiology*. 1987;66(3):405–410.
- You B, Peslin R, Duvivier C, Vu VD, Grilliat JP. Expiratory capnography in asthma: evaluation of various shape indices. *Eur Respir J*. 1994;7(2):318–323.
- Yaron M, Padyk P, Hutsinpillier M, Cairns CB. Utility of the expiratory capnogram in the assessment of bronchospasm. *Ann Emerg Med*. 1996;28(4):403–407.
- Colman Y, Krauss B. Microstream capnography technology: a new approach to an old problem. *J Clin Monit Comput*. 1999;15(6):403–409.
- Hagerty JJ, Kleinman ME, Zurakowski D, Lyons AC, Krauss B. Accuracy of a new low-flow sidestream capnography technology in newborns: a pilot study. *J Perinatol*. 2002;22(3):219–225.
- Sivan Y, Eldadah MK, Cheah TE, Newth CJ. Estimation of arterial carbon dioxide by end-tidal and transcutaneous PCO_2 measurements in ventilated children. *Pediatr Pulmonol*. 1992;12(3):153–157.
- Bhat R, Kim WD, Shukla A, Vidyasagar D. Simultaneous tissue pH and transcutaneous carbon dioxide monitoring in critically ill neonates. *Crit Care Med*. 1981;9(10):744–749.
- Rennie JM. Transcutaneous carbon dioxide monitoring. *Arch Dis Child*. 1990;65(4 Spec No):345–346.
- Rozycki HJ, Sysyn GD, Marshall MK, Malloy R, Wiswell TE. Mainstream end-tidal carbon dioxide monitoring in the neonatal intensive care unit. *Pediatrics*. 1998;101(4 Pt 1):648–653.
- Wu CH, Chou HC, Hsieh WS, Chen WK, Huang PY, Tsao PN. Good estimation of arterial carbon dioxide by end-tidal carbon dioxide monitoring in the neonatal intensive care unit. *Pediatr Pulmonol*. 2003;35(4):292–295.

24. Pascucci RC, Schena JA, Thompson JE. Comparison of a sidestream and mainstream capnometer in infants. *Crit Care Med*. 1989;17(6):560–562.
25. Kugelman A, Zeiger-Aginsky D, Bader D, Shoris I, Riskin A. A novel method of distal end-tidal CO₂ capnography in intubated infants: comparison with arterial CO₂ and with proximal mainstream end-tidal CO₂. *Pediatrics*. 2008;122(6):e1219–e1224.
26. Sakamoto H, Kubota C, Misumi K. Relationship between arterial and end-tidal carbon dioxide pressure during controlled ventilation in porcine neonates. *Exp Anim*. 1996;45(2):195–198.
27. Figueras J, Rodriguez-Miguel JM, Botet F, Thio M, Jimenez R. Changes in TcPCO₂ regarding pulmonary mechanics due to pneumotachometer dead space in ventilated newborns. *J Perinat Med*. 1997; 25(4):333–339.
28. Dreyfuss D, Ricard JD, Saumon G. Ventilator-induced lung injury. In: Tobin MJ, editor. *Principles and practice of mechanical ventilation*. 2nd ed. New York: McGraw-Hill, Inc; 2006:903–930.
29. Coalson JJ. Pathology of new bronchopulmonary dysplasia. *Semin Neonatol*. 2003;8(1):73–81.
30. Donn SM, Sinha SK. Can mechanical ventilation strategies reduce chronic lung disease? *Semin Neonatol*. 2003;8(6):441–448.

Research and Reports in Neonatology

Dovepress

Publish your work in this journal

Research and Reports in Neonatology is an international, peer-reviewed, open access journal publishing original research, reports, editorials, reviews and commentaries on neonatal health. The manuscript management system is completely online and includes a very quick and fair

peer-review system. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.

Submit your manuscript here: <http://www.dovepress.com/research-and-reports-in-neonatology-journal>