

Evaluation of the calculation formulas of the cardio-ankle vascular index used in the Japanese apparatus

Dai Ato 

Gakujutsu Shien Co., Ltd., Tokyo, Japan

This article was published in the following Dove Press journal:
Vascular Health and Risk Management

Background: Recently, coefficients in the equation of cardio-ankle vascular index (CAVI) used in VaSera[®] device were disclosed. This study aimed to simulate the influence of adjusting the coefficients in the equation of CAVI and also aimed to validate the equation.

Methods: The CAVI displayed by VaSera (CAVIs) and the CAVI estimated (CAVies) with fixing the coefficients of the middle range of the heart-ankle stiffness parameter β (ha β) in the equation were compared. Moreover, the heart-ankle pulse wave velocity (haPWV) which corresponds to the low cutoff ha β of 7.348 was estimated in various blood pressure patterns to validate the formula.

Results: The CAVIs was clearly lower than CAVies in the low and the high range of CAVIs. Moreover, it was virtually impossible to obtain the low cutoff ha β of 7.348 by using typical values of haPWV.

Conclusion: The CAVIs in the high-range of VaSera underestimates the original property of stiffness parameter β . Moreover, there will be also a missing information in the equations introduced in the corresponding article, especially in the calculation formula of CAVIs from ha β . Therefore, in order to make the best use of the nature of the stiffness parameter β to be used in VaSera, fixing the coefficients or termination of its use should be considered.

Keywords: brachial-ankle pulse wave velocity, arterial stiffness, arterial compliance, vascular function, peripheral arterial disease, ankle-brachial index

In a recent article published in the *Journal of Atherosclerosis and Thrombosis*, Takahashi et al disclosed the values of coefficients “a” and “b”, which are used to calculate the cardio-ankle vascular index (CAVI) using the VaSera[®] (VS) device.¹ CAVI estimated using VS (CAVIs) is a blood pressure-adjusted product of heart-ankle (ha) pulse wave velocity (PWV); the concept of CAVI is derived from the stiffness parameter β .

The β value for haPWV (ha β) is calculated using the following equation:¹

$$ha\beta = 2\rho \times haPWV^2 \times \ln[SBP/DBP] \div (SBP - DBP)$$

where ρ is blood density (fixed value of 1.05 in VS devices), Ln is natural logarithm, SBP is systolic blood pressure (SBP), and DBP is diastolic blood pressure (DBP).

CAVIs is calculated using the following equation:¹

$$CAVIs = a \times ha\beta + b$$

Regarding this equation, Takahashi et al disclosed that the coefficients “a” and “b” were changed by the ha β level (Table 1) to adjust ha β to Hasegawa-PWV (H-PWV). They explained the reason as follows:

Correspondence: Dai Ato
 Gakujutsu Shien (Academic Support) Co.,
 Ltd., 2-1-17 Nihonbashi, Chuo-ku, Tokyo
 103-0027, Japan
 Tel +81 3 6869 6438
 Email ato.dai@wind.ocn.ne.jp

Table 1 The coefficients of a and b according to $ha\beta$ and CAVIvs

| $ha\beta$ | Low range | Middle range | High range |
|-----------|--------------|----------------------------------|-------------------|
| | <7.34875 | $7.34875 \leq to < 10.30372$ | $10.30372 \leq$ |
| a | 0.85 | 0.658 | 0.432 |
| b | 0.695 | 2.103 | 4.441 |
| CAVIvs | <6.9414375 | $6.9384775 \leq to < 8.88284776$ | $8.89220704 \leq$ |

Note: $CAVIvs = a \times ha\beta + b$.

Abbreviations: ha, heart-ankle; CAVIvs, cardio-ankle vascular index measured by VaSera®.

Because $ha\beta$ is based on PWV squared, whereas H-PWV is based solely on PWV, it is difficult to maintain a high correlation in a wide range of values with one approximate adjustment. For this reason, the portion that coincides with the correlation equation of $ha\beta$ and H-PWV was defined as the middle range. For the upper and lower ranges that were outside the middle range, the coefficients were adjusted so that the difference between H-PWV and CAVI was small throughout the clinical range.¹

Here, a fundamental issue arises. Generally, the logic of the blood pressure (BP) independency of the stiffness parameter β is considered appropriate. However, originally, this hypothesis is to be applied on one arterial location. No logical explanation exists as to why this method is also perfectly valid in the evaluation of the long distant arteries with multiple segments. Nevertheless, we suppose that $ha\beta$ is also BP independent. If we fix the coefficients of “a” and “b”, we can suppose that the characteristics of $ha\beta$ is also reserved in all of the CAVIvs range. However, if coefficients “a” and “b” change according to the $ha\beta$ value, the change in CAVIvs cannot properly reflect the original change in $ha\beta$ when CAVIvs fluctuates across the points where the coefficients change (Figure 1). Therefore, the whole range of CAVIvs can never maintain the property of $ha\beta$ nor stiffness parameter β . In fact, Lim et al demonstrated the difference between CAVIvs and the stiffness parameter β in a BP perturbation study.² In this study, the change in CAVIvs correlated with that in BP, whereas the change in stiffness parameter β measured at the carotid segment did not. This indicates the BP dependency of CAVIvs and the difference between CAVIvs and “real” stiffness parameter β , although direct comparison was impossible due to different segments.

Regarding BP dependency of CAVI, Steppan et al demonstrated the BP dependency of CAVI in a rat model.³ Furthermore, Spronck et al and Segers elegantly proved the residual BP dependency of CAVI.^{4–6} Moreover, the author pointed out a fundamental discrepancy in BP

Presented CAVI

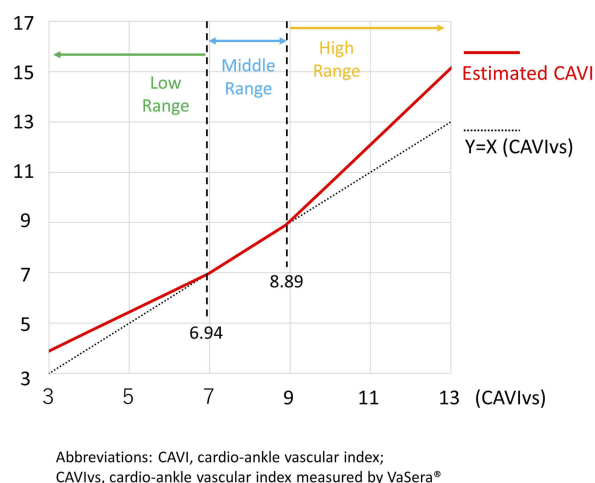


Figure 1 CAVIvs and estimated CAVI if the coefficients in the middle range of $ha\beta$ were fixed in the whole range.

Notes: The horizontal axis means the value of CAVIvs. The vertical axis means the CAVI value according to the methods. The red line shows the CAVI estimated by the coefficients of the middle range fixed.

measured using an oscillometric method from the internal arterial pressure measured with the catheter method.⁷

In addition, there will be also a fault in the equations introduced in the corresponding article.¹ If we calculate $ha\beta$ using typical $haPWV$ value of 7 m/s (and SBP; 115 mmHg, DBP; 75 mmHg), the $ha\beta$ is 1.10. The required $haPWV$ to obtain the low cutoff $ha\beta$ of 7.348 in several BP patterns is summarized in Table 2. The required $haPWV$ values are considered too high for the middle-aged subjects with low cutoff $ha\beta$ and CAVIvs because $haPWV$ is inevitably much lower than $baPWV$ due to the measurement process.⁸ Moreover, according to the study which adopted the same method using $baPWV$ and central BP on the $ha\beta$ equation,⁹ the central SBP was 115 ± 1.0 mmHg (mean \pm standard error (SEM)), the central DBP was 75 ± 1.0 mmHg (SEM), and the $baPWV$ was 16 ± 0.2 m/s (SEM). However, the “brachial-ankle β ” was 5.6 ± 0.1 (SEM), which is much lower than the low cutoff $ha\beta$ of 7.348.

In reality, the SI units should be used for the calculation, ρ should be 1500 kg/m^3 (not 1.05 g/cm^3 or 1.05 kg/L), and the unit of BP should be Pa (using the conversion value of $1 \text{ mmHg} = 133.32 \text{ kg/[m s}^2\text{]})$.¹⁰ Table 3 shows the revision of Table 2 using SI units. The results are plausible for $haPWV$. Therefore, Takahashi et al should have clarified these points.¹

Tabara et al recently found the so-called regression-to-the-mean phenomenon after multivariate adjustment of the longitudinal change in CAVIvs (in about 5 years) in the general population.¹¹ In this study, the most powerful

Table 2 The haPWV to obtain ha β of 7.348 in various BP patterns

| | | | | | | | |
|-------------|--------|--------|--------|--------|--------|--------|--------|
| SBP (mmHg) | 80 | 100 | 120 | 130 | 140 | 160 | 180 |
| DBP (mmHg) | 50 | 60 | 70 | 80 | 90 | 100 | 110 |
| haPWV (m/s) | 14.945 | 16.553 | 18.016 | 18.983 | 19.899 | 21.135 | 22.301 |

Abbreviations: ha, heart-ankle; PWV, pulse wave velocity; BP, blood pressure; SBP, systolic blood pressure; DBP, diastolic blood pressure.

Table 3 The haPWV to obtain ha β of 7.348 in various BP patterns using SI units

| | | | | | | | |
|-------------|----------|--------|----------|----------|----------|----------|----------|
| SBP (mmHg) | 80 | 100 | 120 | 130 | 140 | 160 | 180 |
| DBP (mmHg) | 50 | 60 | 70 | 80 | 90 | 100 | 110 |
| ↓ | ↓ | ↓ | ↓ | ↓ | ↓ | ↓ | ↓ |
| SBP (Pa) | 10,665.6 | 13,332 | 15,998.4 | 17,331.6 | 18,664.8 | 21,331.2 | 23,997.6 |
| DBP (Pa) | 6666 | 7999.2 | 9332.4 | 10,665.6 | 11,998.8 | 13,332 | 14,665.2 |
| haPWV (m/s) | 5.457 | 6.044 | 6.578 | 6.931 | 7.266 | 7.717 | 8.143 |

Notes: 1 mmHg is converted to 133.32 Pa. ρ is 1050 kg/m³.

Abbreviations: ha, heart-ankle; PWV, pulse wave velocity; BP, blood pressure; SBP, systolic blood pressure; DBP, diastolic blood pressure.

independent determinant of the change in CAVIs (Δ CAVIs) was the baseline CAVIs (standardized coefficient, -0.590 ; $P < 0.001$). Moreover, Δ CAVIs was approximately -0.3 in the subjects with a baseline CAVIs of ≥ 9.5 , which indicated a decrease in CAVIs in the multivariate adjusted model. The reason for these phenomena may be partly explained by the decrease in the coefficient “a” in the high range of ha β compared with that in the middle range of ha β .

Therefore, if we continue to use CAVIs, we must be aware of the difference in CAVIs from that of ha β when CAVIs changes across the designated low and high points of CAVIs (6.94 and 8.89, respectively). We must also recognize the substantial underestimation of the significance of high CAVIs (>8.89) in regard to the original significance of the stiffness parameter β . Moreover, any fault in the corresponding article¹ as pointed out above must be immediately amended.

Finally, if the original nature of stiffness β is to be properly adopted for haPWV in the VS device, the author suggests revalidation of the previous and upcoming data by fixing the coefficients or terminating the use of coefficients “a” and “b”. This will be the best way to use the concept of stiffness parameter β on PWV indices not only for ourselves but also for the researchers and the patients in the future. Grillo et al suggest that the calculation of β -stiffness index from PWV and BP-values is an interesting evolution that could overcome limitations and ambiguities derived from the BP dependency of the properties of the arterial wall, although the way of calculating this parameter is still debated.¹² Combined use of the CAVI-0

method can be considered as well.^{4–7} Recently, Spronck et al presented an easy and useful method (using simple software, either Microsoft® Excel or PDF) to convert CAVIs to CAVI0, which will greatly help in the simultaneous research on CAVIs and CAVI0.¹³ The use of CAVIs has spread widely. However, around 15 years have passed since it was produced, and it is used as a parameter only in VaSera. Conversely, adaptation of the stiffness β method on PWVs without using coefficients is the simplest method and will be available for the foreseeable future. In this situation, some difficulty is expected to emerge in the compatibility between CAVIs and other PWV-derived stiffness β . As adequate data have been accumulated using VS, estimation of CAVI no longer has to rely on H-PWV data with deteriorating the nature of stiffness parameter β .

Acknowledgment

The author appreciates the researchers and participants of the preceding studies.

Disclosure

Dai Ato is a former employee of Fukuda Colin (formerly Omron Colin, Nippon Colin) Co., Ltd., a distributor of Vascular Profiler® (form PWV/ABI, BP-203RPE series). Dai Ato is an independent researcher and wrote this article as an academic activity based on the guaranteed right of freedom in academia for the Japanese (Article 23) and on the supreme law provided in Article 98 of the Constitution of Japan. Dai Ato reports no other conflicts of interest in this work.

References

1. Takahashi K, Yamamoto T, Tsuda S, et al. Coefficients in the CAVI equation and the comparison between CAVI with and without the coefficients using clinical data. *J Atheroscler Thromb*. 2019;26(5):465–475. doi:10.5551/jat.44834
2. Lim J, Pearman ME, Park W, Alkatan M, Machin DR, Tanaka H. Impact of blood pressure perturbations on arterial stiffness. *Am J Physiol Regul Integr Comp Physiol*. 2015;309(12):R1540–R1545. doi:10.1152/ajpregu.00368.2015
3. Steppan J, Sikka G, Hori D, et al. Seeking a blood pressure-independent measure of vascular properties. *Hypertens Res*. 2016;39(1):27–38. doi:10.1038/hr.2015.109
4. Spronck B, Avolio AP, Tan I, Butlin M, Reesink KD, Delhaas T. Arterial stiffness index beta and cardio-ankle vascular index inherently depend on blood pressure but can be readily corrected. *J Hypertens*. 2017;35(1):98–104. doi:10.1097/HJH.0000000000001132
5. Segers P. A lesson in vigilance: pressure dependency of a presumed pressure-independent index of arterial stiffness. *J Hypertens*. 2017;35(1):33–35. doi:10.1097/HJH.0000000000001139
6. Spronck B, Avolio AP, Tan I, Butlin M, Reesink KD, Delhaas T. Reply: physics cannot be disputed. *J Hypertens*. 2017;35(7):1523–1525. doi:10.1097/HJH.0000000000001350
7. Ato D. Brachial-ankle pulse wave velocity, cardio-ankle vascular index, and prognosis. *Vasc Health Risk Manag*. 2018;24(14):321–348. doi:10.2147/VHRM.S179366
8. Sugawara J, Hayashi K, Tanaka H. Arterial path length estimation on brachial-ankle pulse wave velocity: validity of height-based formulas. *J Hypertens*. 2014;32(4):881–889. doi:10.1097/HJH.0000000000000114
9. Kim T, Lee CS, Lee SD, et al. Impacts of comorbidities on the association between arterial stiffness and obstructive sleep apnea in the elderly. *Respiration*. 2015;89(4):304–311. doi:10.1159/000371768
10. Spronck B, Mestanik M, Tonhajzerova I, et al. Direct means of obtaining CAVI0-a corrected cardio-ankle vascular stiffness index (CAVI)-from conventional CAVI measurements or their underlying variables. *Physiol Meas*. 2017;38(10):N128–N137. doi:10.1088/1361-6579/aa8981
11. Tabara Y, Setoh K, Kawaguchi T, et al. Factors affecting longitudinal changes in cardio-ankle vascular index in a large general population: the Nagahama study. *J Hypertens*. 2018;36(5):1147–1153. doi:10.1097/HJH.0000000000001672
12. Grillo A, Salvi P. Cardio-ankle vascular index and carotid-femoral pulse wave velocity: limits and strengths. *J Hypertens*. 2018;36(4):759–764. doi:10.1097/HJH.0000000000001666
13. Spronck B, Mestanik M, Tonhajzerova I, et al. Easy conversion of cardio-ankle vascular index into CAVI0: influence of scale coefficients. *J Hypertens*. 2019;37(9):1913–1914. doi:10.1097/HJH.0000000000002166

Vascular Health and Risk Management

Dovepress

Publish your work in this journal

Vascular Health and Risk Management is an international, peer-reviewed journal of therapeutics and risk management, focusing on concise rapid reporting of clinical studies on the processes involved in the maintenance of vascular health; the monitoring, prevention and treatment of vascular disease and its sequelae; and the involvement

of metabolic disorders, particularly diabetes. This journal is indexed on PubMed Central and MedLine. The manuscript management system is completely online and includes a very quick and fair peer-review system, which is all easy to use. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.

Submit your manuscript here: <https://www.dovepress.com/vascular-health-and-risk-management-journal>