

Progress in Nanomaterials-Based Optical and Electrochemical Methods for the Assays of Exosomes

Xiaohua Ma¹
Yuanqiang Hao¹
Lin Liu^{1,2}

¹Henan Key Laboratory of Biomolecular Recognition and Sensing, Shangqiu Normal University, Shangqiu, Henan, 476000, People's Republic of China;
²College of Chemistry and Chemical Engineering, Anyang Normal University, Anyang, Henan, 455000, People's Republic of China

Abstract: Exosomes with diameters of 30–150 nm are small membrane-bound vesicles secreted by a variety of cells. They play an important role in many biological processes, such as tumor-related immune response and intercellular signal transduction. Exosomes have been considered as emerging and noninvasive biomarkers for cancer diagnosis. Recently, a large number of optical and electrochemical biosensors have been proposed for sensitive detection of exosomes. To meet the increasing demands for ultrasensitive detection, nanomaterials have been integrated with various techniques as powerful components. Because of their intrinsic merits of biological compatibility, excellent physicochemical features and unique catalytic ability, nanomaterials have significantly improved the analytical performances of exosome biosensors. In this review, we summarized the recent progress in nanomaterials-based biosensors for the detection of cancer-derived exosomes, including fluorescence, colorimetry, surface plasmon resonance spectroscopy, surface enhanced Raman scattering spectroscopy, electrochemistry, electrochemiluminescence and so on.

Keywords: exosomes, nanomaterials, circulating tumor biomarkers, electrochemical biosensor, optical biosensor

Introduction

Cancer is the main cause of death, and its occurrence and development is a gradual and complicated process. Early diagnosis and treatment of cancer can enormously improve the survival chance of cancer patients. Extracellular vesicles (EVs) are secreted by various cell types and circulate in different body fluids. They were first discovered as “cell junks” about 40 years ago.^{1,2} The lack of specific and reliable markers makes the clear assignation of EV subtypes extraordinarily difficult. According to operational terms for EV subtypes proposed by the International Society for Extracellular Vesicles (ISEV), EVs can be classified into three groups based on their size: exosomes, small EVs (sEVs) (< 200 nm), medium EVs (mEVs), and large EVs (lEVs).³ Exosomes are nanosized extracellular vesicles (EVs) (30–200 nm). For the convenience of the reader, this review used a relatively broad term of “exosomes” to refer to a heterogeneous mixture of sEVs less than 200 nm in size because it is increasingly utilized in bioassays.⁴ Compared to circulating tumor cells and circulating DNA, exosomes exist in body fluids (such as serum, urine and ascites) with higher abundance and stability.⁵ Emerging evidences suggest that most types of cancer secrete large numbers of exosomes that carry abundant molecular information stemming from parent tumor cells, including nucleic acids, proteins, bioactive lipids and metabolites.^{6,7}

Correspondence: Yuanqiang Hao; Lin Liu
Email hao0736@163.com;
liulin82414@aliyun.com

Exosomes can act as cellular messengers to deliver information between cells via endocytosis.^{8,9} They also play a key role in cancer metastasis and progression in the tumor microenvironment.^{10,11} Moreover, various unique cargos in exosomes represent meaningful physiological and pathological states of diseases.^{12,13} Therefore, exosomes have been recognized as the most reliable non-invasive biomarkers for the early diagnosis and cure of cancers.^{14–17}

Various exosomes-containing complex biological fluids have a plenty of nonvesicular macromolecules, such as proteins, proteases, nuclease and RNA complexes, which may interfere with the analysis of exosomes. For example, proteases and nuclease can digest the biorecognition elements such as antibodies and aptamers. Thus, the growing interests in exosomes and their potential applications in cancer detection have pushed researchers to develop various isolation and detection techniques. Normally, conventional isolation techniques, including ultracentrifugation, density gradient centrifugation and ultrafiltration, are mainly based on the physical properties of exosomes (eg size and density).^{5,18} However, these techniques confront of some problems, such as low purity, tedious procedures and requirement of expensive instruments. Traditional detection techniques utilized to quantify the isolated exosomes include nanoparticle tracking analysis (NTA), flow cytometry, Western blot, dynamic light scattering, scanning electron microscope (SEM), and transmission electron microscope (TEM).^{2,19–22} Although these methods have been popularly used, the problems of low reproducibility, time consuming, large sample demand and low sensitivity limit their further applications.

Over the past years, many types of proteins, such as tetraspanins (eg CD9, CD63, CD81 and CD82), adhesion molecules (eg integrins and lactadherin) and lipid rafts (eg cholesterol, phosphatidylserine and ceramide), have been found on the membrane of all types of exosomes.^{23,24} These biomolecules can be utilized as the targets for the detection of total exosomes. However, exosomes derived from various tumor cells exhibit different cancers-associated antigens on the surface. These distinct antigens have been used as the biomarkers for the determination of certain cancer-derived exosomes.²⁵ For example, MCF-7-secreted exosomes with highly expressed MUC1 on the surface.²⁶ Protein tyrosine kinase 7 and CD147 are over-expressed on the surface of human leukemic lymphoblasts (CCRF-CEM) and colorectal cancer cellular exosomes, respectively.^{27,28} These proteins are the promising markers

for the isolation and detection of exosomes with the aid of biorecognition elements.^{29,30} By modifying magnetic beads (MBs), chips or microfluidics with antibodies toward exosome membrane markers, immunoaffinity-capture-based techniques are proposed for the isolation and enrichment of exosomes with high selectivity and specificity as well as intact biological activity.^{23,31–44} However, the expensive cost and instability of antibodies limit their practical applications. Aptamers and peptides are screened to act as biorecognition elements for the isolation and detection of exosomes by the virtue of low cost, small size and relatively excellent stability.^{45–47} Besides, exosomal glycans provide a valuable route to label exosomes through the interaction of lectin and glycan.^{48,49} Lipophilic cholesterol anchors can penetrate into the lipid bilayers for membrane modification, which have been regarded as the promising candidates for labeling of exosomes.^{50,51} In contrast to physical property-based isolation techniques, affinity-based isolation techniques exhibit much higher enrichment efficiency, facilitating the sensitive detection of exosomes.

In recent years, numerous novel biosensors with high sensitivity and efficiency have been established for the determination of exosomes by specific recognition, including colorimetry, fluorescence, surface plasmon resonance (SPR), surface enhanced Raman scattering (SERS) spectroscopy, mass spectrometry and electrochemical, electrochemiluminescent (ECL) and photoelectrochemical (PEC) assays.^{4,52–59} Moreover, many works based on microfluidic devices implemented with optical or electrochemical techniques have been reported for the comprehensive assays of exosomes.^{60–64}

With the growing development of nanotechnology, myriad nanomaterials and nanostructures have made a great impact on biosensing. Significant advances have made it possible to controllably prepare nanomaterials with various chemical composition, morphology and physicochemical characteristics. For example, nanomaterials with wonderful luminescence properties have been an important alternative to traditional dyes in optical assays, because of their excellent merits of adjustable emission wavelength, high luminescence quantum yield and good photostability. Thanks to the interesting size and shape-dependent localized surface plasmon resonance phenomenon, noble metal nanoparticles (NPs), especially gold and silver, have been widely used to enhance the signal intensity in SPR and SERS assays. Carbon-based nanomaterials (eg, carbon nanotubes and graphene oxide) with a high

surface-to-volume ratio and high electrical conductivity are always employed for electrode modification to accelerate the electron transfer and increase the electrode surface area. Moreover, recently, the photothermal and enzyme-mimic properties of nanomaterials have gained considerable interest toward the development of portable bioassays. Various nanomaterials-based signal amplification strategies, coupled with different detection techniques, have been developed for the ultrasensitive detection of biomolecules, including DNA/RNA, proteins, exosomes and cells. In exosomes detection, there are two mainly objectives, including improving the capture of exosomes and enhancing the performance of detection methods. For the former, magnetic beads (MBs) as the classical materials have been increasingly used to selectively capture exosomes from clinical samples, when being decorated with antibodies or aptamers.

In this review, the recent progress in nanomaterials-based biosensors for exosome detection was comprehensively summarized. The detection techniques mainly cover optical and electrochemical assays (Tables 1 and 2). Nanomaterials are involved in semiconductor quantum dots (QDs), metal NPs, metal oxides and sulfides, and carbon-based nanomaterials. The intent of this review is to impart insights into the versatile roles of nanomaterials in assays, and illustrate their potential benefits in further applications.

Nanomaterials-Based Optical Biosensors for Exosome Detection Fluorescence Biosensors

Fluorescence biosensors have great advantages of simple operation, comparable sensitivity, and multiplex target detection capability. Exosome can be labeled with dyes or dye-modified biorecognition elements through various targeting strategies and then determined by fluorescence imaging or spectroscopy.^{50,65–72} However, the low fluorescence intensities of dyes always limits the sensitivity for exosome detection.⁷³ Thus, several signal amplification strategies have been proposed to improve the detection sensitivity.^{74,75} For example, β -galactosidase-labeled antibody was used to label the captured exosomes in which β -galactosidase acted as the reporter enzyme to catalyze the decomposition of fluorescein-di- β -D-galactopyranoside, generating a strong fluorescence signal.^{41,76} Combined with nano-interface-based microfluidic platforms, exosomes were effectively enriched and sensitively detected.

For homogeneous fluorescence detection, it is one of the most powerful strategies to convert the detection of exosomes into the detection of DNA or others, generally producing a “one-to-many” amplification effect.^{77–81} Owing to the flexible structure, the corresponding DNA can be ultrasensitively and homogeneously detected by previously reported DNA-based signal amplification methods, such as terminal deoxynucleotidyl transferase (TdT)-mediated polymerization and hybridization chain reaction (HCR).^{82–89} For example, Gao et al reported a dual signal amplification method for indirect detection of exosomes based on the catalytic hairpin DNA cascade reaction (HDCR) and the self-assembly of DNA dendrimer on the surface of gold nanoparticles (Au NPs).⁹⁰ In this work, streptavidin (SA)-modified MBs were labeled with biotin-modified CD63 aptamer and then bound with probe S through the hybridization. After the addition of exosomes, aptamers bound with CD63 on exosomes and the probe S was released to trigger the HDCR on the nanoparticle surface. Then, the opened metastable hairpin (HP) DNA probes captured the fluorescently-labeled DNA dendrimers. After several rounds of Y-shaped DNA assembly, the complexes of AuNPs, HP and DNA dendrimers were separated. With the aid of β -mercaptoethanol, the fluorescently-labeled dendrimers were released and the fluorescence signal was recorded for the determination of exosomes. This method showed an increased signal-to-noise ratio and had a linear detection range of $1.75 \times 10^3 - 7.0 \times 10^6$ particles/ μ L. Pan et al reported a steric hindrance-controlled signal-amplified fluorescent strategy for exosome detection.⁹¹ In the absence of exosome, cholesterol-conjugated DNA 1 could hybridize with SA-modified DNA 2 into dsDNA with blunt ends. The formed dsDNA could not be recognized and extended by TdT enzyme because of the absence of single-stranded initiator (more than three deoxynucleotide residues). However, when exosomes were added, DNA 1 was inserted into the lipid membrane through the hydrophobic interaction between cholesterol and lipid bilayer. The huge steric hindrance of exosomes strongly inhibited the hybridization of DNA 1 and SA-modified DNA 2. Therefore, SA-modified DNA 2 could be extended by TdT enzyme to generate abundant G-quadruplex structures, increasing the fluorescence intensity. The “signal-on” method maintained high sensitivity and excellent selectivity for the assay of complex samples. Li et al developed a reversible nanoplatform for fluorescent detection of urinary exosomes by using a superparamagnetic conjunction and molecular beacon.⁹² As shown in Figure 1, prostate specific membrane antigen (PSMA) aptamer was modified on the

Table 1 An Overview on Nanomaterials-Based Optical Methods for Exosome Detection

Methods	Type of Nanomaterials	Functions	Cancer Types	Target Biomarkers	Response Time (min)	Detection Limit (Particles/ μ L)	Linear Range (Particles/ μ L)	Ref.
Fluorescence	Biorecognition elements-modified MNPs	Capturing exosomes and transforming the detection of exosomes into the detection of DNA with DNA-based signal amplification	Liver cancer	CD63	Not reported	0.1	$1-1 \times 10^4$	[83]
			Not reported	CD63 and lipid bilayer	160	1.29×10^3	$5.5 \times 10^3-1.1 \times 10^7$	[84]
			Lung cancer	CD63	65	1×10^5	$1 \times 10^7-1 \times 10^9$	[85]
			Lung cancer	CD63	95	0.1	$0.3-1 \times 10^4$	[86]
			Liver cancer	CD63	255	1.16×10^3	$1.75 \times 10^3-7 \times 10^6$	[90]
	QDs	Fluorescence labels	Cervical cancer	CD63 and lipid bilayer	245	480	$1.66 \times 10^3-1.66 \times 10^6$	[91]
			Prostate cancer	PSMA	210	1×10^2	$1 \times 10^3-1 \times 10^8$	[92]
			Lung cancer	EpCAM	60	0.013	$5 \times 10^2-5 \times 10^9$	[94]
			Oral squamous Cell carcinoma	CD63	30	5×10^2	$5.0 \times 10^2-1.0 \times 10^5$	[95]
			Pancreatic cancer	GPC-1	90	Not reported	$1.0 \times 10^4-1.0 \times 10^6$	[96]
	CuNPs	Nanoquenchers	Human tongue squamous cell carcinoma	Lipid bilayer	65	2×10^3	$4 \times 10^3-2 \times 10^5$	[97]
			Liver cancer	CD63 and lipid bilayer	120	4.8×10^4	$7.5 \times 10^4-1.5 \times 10^7$	[98]
			Leukemia cell	CD63 and nucleolin	180	1×10^2	$1 \times 10^3-1 \times 10^5$	[88]
			Breast cancer	PSMA	40	1.6×10^2	$1.6 \times 10^2-1.6 \times 10^5$	[101]
			Colorectal cancer	CD63 and EpCAM	40	2.1×10^4	$3 \times 10^4-6 \times 10^5$	[102]
	MoS ₂ -MWCNTs	Nanoquenchers and luminescent emitters	Breast cancer	GPC-1	128	6.56×10^4	$7.8 \times 10^4-3.9 \times 10^9$	[103]
			Breast cancer	CD63	70	1.48×10^3	$0-1.11 \times 10^4$	[104]
			Breast cancer	CD63	70	1.4	$10-1 \times 10^6$	[105]
			Breast cancer	CD63	250	8.2	$20-2.0 \times 10^6$	[99]
			Breast cancer	CD63	250	8.2	$20-2.0 \times 10^6$	[99]

Colorimetry	AuNPs	Nanocarriers for enzymes	Colorectal cancer	A33 and EpCAM	220	6.7×10^3	9.75×10^3 – 1.95×10^6	[114]
	AuNPs	Color indicators	Nasopharyngeal carcinoma	CD63, CD9, CD81, LMP1 and EGFR	120	0.1	0.1 – 1×10^5	[122]
	AuNRs		Breast cancer	CD63 and lipid bilayer	Not reported	1.6×10^2	1.4×10^3 – 2.8×10^5	[127]
	Au NBP@ MnO ₂ NSs		Breast cancer	CD63	155	1.35×10^2	8.5×10^2 – 8.5×10^4	[128]
	C-IONPs	Nanozymes	Ovarian cancer	CD63		1.25×10^3	6.25×10^2 – 1.0×10^4	[129]
	g-C ₃ N ₄ nanosheets	Peroxidase-mimetic enzyme	Breast cancer	CD63	30	1.352×10^6	1.9×10^6 – 3.38×10^7	[132]
	SWCNTs		Breast cancer	CD63	40	5.2×10^5	1.84×10^6 – 2.21×10^7	[133]
	CuCo ₂ O ₄ nanorods		Breast cancer	CD63	160	4.5×10^3	5.6×10^4 – 8.9×10^5	[134]
	GO	Chip substrate	Lung cancer	PD-L1	50	0.02	10 – 1.0×10^5	[145]
	MNPs	Nanotags	Lung cancer	CD63, EGFR and EpCAM	55	2.37×10^4	3.125×10^4 – 100×10^4	[148]
SERS	AuNPs		Breast cancer	CD63	155	5	Not reported	[151]
	AuNPs	Raman reporters with LSPR	Pancreatic cancer	CD63, GPC-1, EpCAM and CD44V6	150	Not reported	Not reported	[164]
	Polydopamine-encapsulated Au@Ag NPs		Pancreatic cancer	CD63, GPC-1, EGFR, EpCAM, and MIF	150	Not reported	0.544–27.2	[161]
	AuNS@4-MBA@Au		Hepatocellular Carcinoma	CD9 and lipid bilayer	50	27	40 – 4.0×10^7	[162]
	Gold-silver-silver core shell-shell nanoporepangs		Hepatocellular Carcinoma	PSMA, Her2 and AFP	120	35	1 – 1×10^7	[168]
	TP-DNA@AuNPs	Electromagnetic hot spots to enhance Raman signals	Breast cancer	EpCAM	150	110	1×10^3 – 1×10^7	[169]

Abbreviations: QDs, quantum dots; CuNPs, copper nanoparticles; AuNPs, gold nanoparticles; AuNRs, gold nanorods; UCNPs, upconversion nanoparticles; Au NBP@MnO₂ NSs, gold nanobipyramid@MnO₂ nanosheet nanostructures; C-IONPs, carboxyl group-functionalized iron oxide nanoparticles; SWCNTs, single-walled carbon nanotubes; Au@PDA NPs, polydopamine-functionalized gold nanoparticle; TP-DNA, triangular pyramidal DNA; AuNS@4-MBA@Au, gold nanostar@4-mercaptopbenzoic acid@nanoshell structures; PSMA, prostate-specific membrane antigen; GPC-1, glypican-1; EpCAM, epithelial cell adhesion molecule; LMP1, latent membrane protein 1; EGFR, epidermal growth factor receptor; PD-L1, programmed death ligand-1; CD44V6, CD44 variant isoform 6; MIF, migration inhibitory factor.

Table 2 An Overview on Nanomaterials-Based Electrochemical Methods for Exosome Detection

Methods	Type of Nanomaterials	Functions	Cancer Types	Target Biomarkers	Response Time (min)	Detection Limit (Particles/ μ L)	Linear Range (Particles/ μ L)	Ref.
Electrochemistry (direct detection)	AuNPs	Improving the large surface area, accelerating electrical conductivity and facilitating the immobilization of biorecognition elements	Breast cancer	CD63	180	4.82×10^2	$5 \times 10^2 - 5 \times 10^3$	[181]
	BPNSs and MOFs		Breast cancer	CD63	Not reported	1×10^2	$1.3 \times 10^2 - 2.6 \times 10^5$	[182]
Electrochemistry (sandwich detection)	AuNPs	Nanocarriers for enzymes, electroactive molecules	Liver cancer	CD63	255	16.6	$21.6 - 7.5 \times 10^4$	[189]
	Zr-MOF		Glioblastoma	EGFR, EGFRVIII, and phosphate groups outside of exosomes	150	7.83×10^3	$9.5 \times 10^3 - 1.9 \times 10^7$	[190]
	Zr-MOF and ZIF-8		Breast cancer	CD63 and phosphate groups outside of exosomes	190	0.3	$1 - 1 \times 10^5$	[191]
	ZIF-8		Breast cancer	CD63 and PD-L1	245	0.334	$1 - 1 \times 10^7$	[192]
	COFs@Au NPs		Colorectal cancer	CD63 and amino acid residues outside of exosomes	170	1.6×10^2	$5 \times 10^2 - 5 \times 10^7$	[193]
	Au-NPFe ₂ O ₃ NC		Placental choriocarcinoma	CD63 and PLAP	90	1	$1 - 1 \times 10^4$	[194]
	Ti ₃ C ₂ MXene@PB		Ovarian cancer	CD63	120	2.29×10^2	$5 \times 10^2 - 5.0 \times 10^5$	[195]
	CdSe QDs		Colorectal adenocarcinoma	CD63, HER-2 and FAM134B	130	1×10^2	$1 \times 10^2 - 1 \times 10^7$	[196]

Electrochemiluminescence	Ru(II) markers-loaded SiNPs	Nanomaterials acts as nanocarriers for molecules	Hepatocellular carcinoma	CD63	120	60	$2 \times 10^2 - 7.5 \times 10^4$	[212]
	CdS:Eu QDs	Electrochemiluminescence emitter	Breast cancer	CD63	240	74.1	$3.4 \times 10^2 - 1.7 \times 10^4$	[210]
	CdS QDs@CaCO ₃		Breast cancer	EpCAM	180	21	$50 - 1 \times 10^5$	[212]
	g-C ₃ N ₄ @Galinstan-PDA		Cervical cancer	GPC-I	120	31	$50 - 1 \times 10^5$	[211]
	BPQDs@ Ti ₃ C ₂ MXene	Coreactants	Breast cancer	CD63 and EpCAM	100	37	$1.1 \times 10^2 - 1.1 \times 10^7$	[214]
	AuNPs@ Ti ₃ C ₂ MXene	Nanocatalysts	Cervical cancer	CD63	240	30	$1 \times 10^2 - 1 \times 10^5$	[215]
	Ti ₃ C ₂ MXene		Breast cancer	EpCAM	240	1.25×10^2	$5 \times 10^2 - 5 \times 10^6$	[213]
	AuNPs@ g-C ₃ N ₄		Ovarian cancer	phosphatidylserine	120	39	$1 \times 10^2 - 1 \times 10^7$	[216]

Abbreviations: BPNs, black phosphorus nanosheets; AuNPs, gold nanoparticles; MOFs, metal organic frameworks; Au-NPFe₂O₃NC, gold-loaded ferric oxide nanocubes; PB, Prussian blue; QDs, quantum dots; PDA, polydopamine; BPQDs, black phosphorus quantum dots; EGFR, epidermal growth factor receptor; EGFRvIII, epidermal growth factor receptor variant (v) III mutation; PD-L1, programmed death ligand-1; PLAP, placental alkaline phosphatase; EpCAM, epithelial cell adhesion molecule; GPC-I, glycican-I.

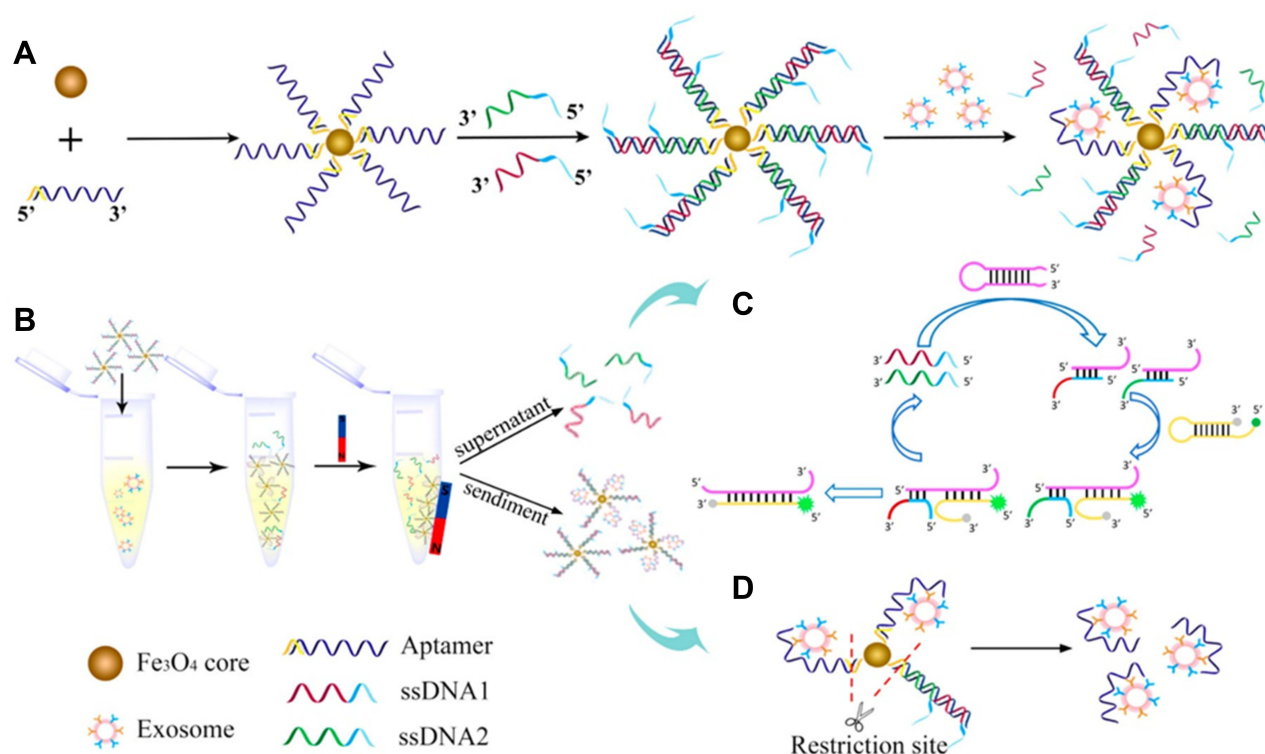


Figure 1 Schematic of SMC-MB platform. (A) Construction of SMC-MB platform. (B) Procedure of SMC-MB platform in exosomes analysis. (C) Principle of nonenzymatic amplification cycle. (D) Exosomes purification by restriction enzyme. Reprinted with permission from Li P, Yu X, Han W, et al. Ultrasensitive and reversible nanoplateform of urinary exosomes for prostate cancer diagnosis. *ACS Sens.* 2019;4:1433–1441. Copyright 2019 American Chemical Society.⁹²

surface of superparamagnetic NPs and then hybridized with two ssDNA strands with the decreased hybridization energy. Exosome bound to the aptamer with high affinity resulted in the release of double amounts of ssDNA to initiate the amplification cycle with two hairpin DNA strands. Molecular beacon HP2 was opened and the fluorescence of probe was recovered. The two released ssDNA sequences with low concentration initiated the amplification cycle with two hairpin DNA strands. Numerous molecular beacon HP2 were opened and the fluorescence of probe was recovered. The detection limit of this method was 100 particles/ μL for the assay of urine samples.

In contrast to traditional fluorescence dyes, QDs possess size/component-tunable luminescence and excellent resistance against photobleaching, which have been widely applied in bioimaging, luminescent biolabels and light-emitting devices.^{93,94} Wu et al proposed a “one-step” strategy for the detection of exosomes using aptamers as the biorecognition elements and QDs as the signal-amplified reporters (Figure 2A).⁹⁵ CD63 aptamer was anchored on the surface of magnetic microspheres (MMs) and tethered to the self-assembled DNA concatemers. Then, streptavidin (SA)-conjugated QDs were used to label the biotin-modified DNA

concatemers. Exosome preferentially bound to the aptamer and induced the release of QDs-labeled DNA concatemers. After the magnetic separation, the fluorescence signal in the supernatant was monitored for exosome detection. Zhang et al prepared a biomimetic periodic nanostructure-based diagnostic biochip for exosome detection using QDs.⁹⁶ As displayed in Figure 2B, glypican-1 (GPC1) antibody-modified QDs were utilized to label exosomes. When the solution was dropped on the photonic crystals-coated biochip, the fluorescence was significantly amplified. In addition, QDs-embedded silica NPs were also used to extracellular vesicles via membrane biotinylation strategy in lateral flow assay (LFA).⁹⁷

Metal nanoclusters (such as Au, Ag and Cu) with ultrasmall size possess excellent fluorescent properties. Ye’s group proposed a copper-mediated signal-amplified method to quantify exosomes (Figure 2C).⁹⁸ In this work, cholesterol-modified MBs were used to capture exosomes via the hydrophobic interaction between cholesterol group and lipid membrane. CD63 aptamer-modified CuO NPs were utilized to label exosome and Cu^{2+} ions were released under acidolysis after the magnetic separation. Numerous released Cu^{2+} ions could be reduced into

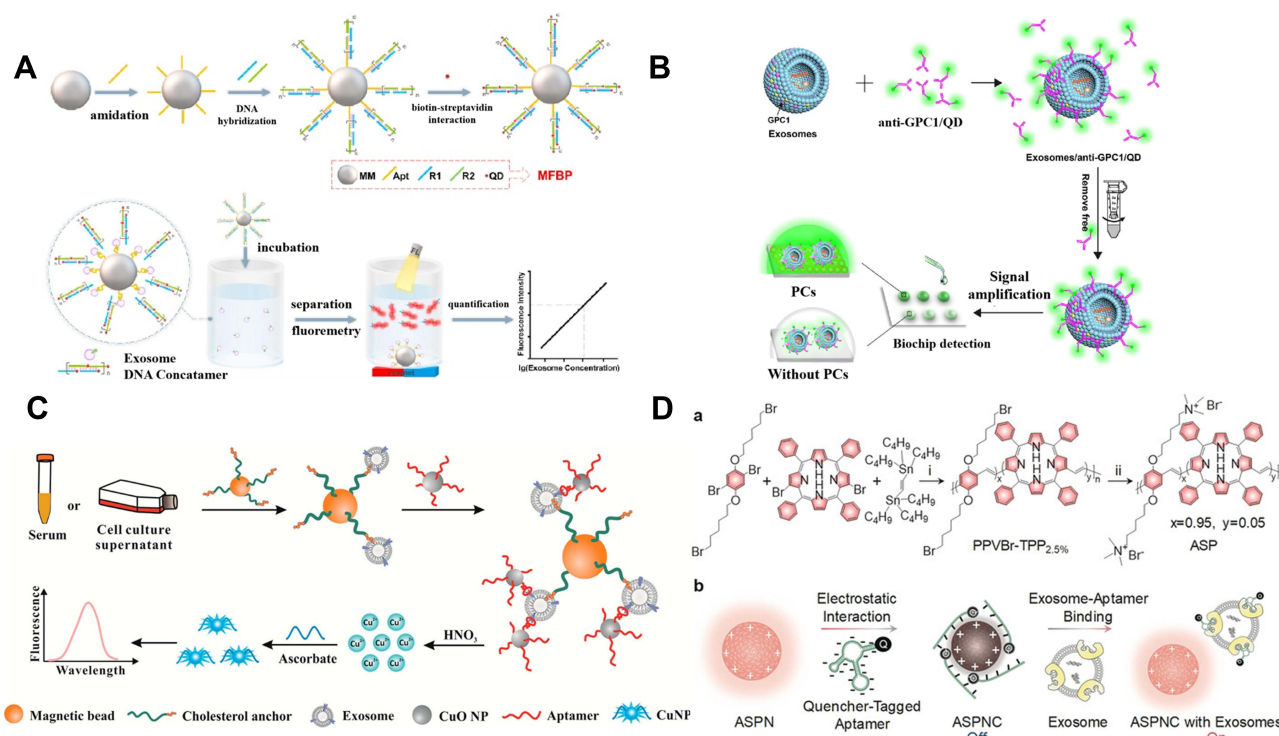


Figure 2 (A) Schematic of magnetic and fluorescent bio-probes (MFBP) constructing process and sensing principle of MFBP-based quantification of exosomes. Reprinted with permission from Wu M, Chen Z, Xie Q, et al. One-step quantification of salivary exosomes based on combined aptamer recognition and quantum dot signal amplification. *Biosens Bioelectron.* 2021;171:112733–112742. Copyright 2021 Elsevier B.V.⁹⁵ (B) Schematic of photonic crystals-assisted signal amplification for measurement of tumor-derived exosomes. Reprinted with permission from Zhang J, Zhu Y, Shi J, et al. Sensitive signal amplifying a diagnostic biochip based on a biomimetic periodic nanostructure for detecting cancer exosomes. *ACS Appl Mater Interfaces.* 2020;12:33473–33482. Copyright 2020 American Chemical Society.⁹⁶ (C) Schematic of the proposed method for exosome detection based on a copper-mediated signal amplification strategy. Reprinted with permission from He F, Wang J, Yin BC, Ye BC. Quantification of exosome based on a copper-mediated signal amplification strategy. *Anal Chem.* 2018;90:8072–8079. Copyright 2018 American Chemical Society.⁹⁸ (D) Schematic of design and sensing mechanism of ASPNC. (a) Synthetic route of ASP. Reagents and conditions: i) tris(dibenzylideneacetone)dipalladium(0) [$\text{Pd}(\text{dba})_3$], tri (*p*-tolyl)phosphine (TPTP), chlorobenzene, 100°C, 24 h; ii) trimethylamine, tetrahydrofuran (THF), methanol, 24 h. (b) Illustration of the formation of ASPNC and the afterglow detection of exosomes. Reprinted with permission from Lyu Y, Cui D, Huang J, Fan W, Miao Y, Pu K. Near-infrared afterglow semiconducting nano-polycomplexes for the multiplex differentiation of cancer exosomes. *Angew Chem Int Ed.* 2019;58:4983–4987. Copyright 2019 Wiley-VCH.⁶⁹

fluorescent Cu nanoclusters with poly(thymine) as the template. Furthermore, Lyu et al constructed a luminescent nanosensor for exosome detection by using an afterglow semiconducting polyelectrolyte nanocomplex (ASPNC).⁶⁹ As displayed in Figure 2D, the backbone of poly(phenylenevinylene) (PPV) modified with cationic quaternary ammonium groups was conjugated with tetraphenylporphyrin (TPP) for the red-shift of the emission and the enhancement of the afterglow signal. The positively charged ASPNC could adsorb the quencher the black hole quencher 2 (BHQ-2)-labeled aptamer through the electrostatic interaction and the afterglow and fluorescence signal were quenched through the efficient electron transfer between the PPV backbone and BHQ-2. In the presence of exosomes, the specific and strong affinity between exosomal protein and BHQ-2-labeled aptamer resulted in the desorption of aptamer from the ASPNC. Consequently, the afterglow and fluorescence signal were restored.

Nanomaterials with excellent fluorescent quenching ability are attractive to develop “on-off” biosensors. Zhang’s reported a dual-signal amplification platform for the analysis of leukemia-derived exosomes based on rolling circle amplification (RCA) and nicking endonuclease-assisted target recycling.⁸⁸ In addition, Yu et al proposed a 3D DNA motor-based platform for the detection of exosomes by using AuNPs as the tracks.⁹⁹ As shown in Figure 3A, AuNPs were modified with fluorescein-labeled substrate strands and aptamer-locked motor strands. In the presence of exosomes, the aptamer bound to the target protein and the motor strand was unlocked to trigger the DNA motor process. Powered by restriction endonuclease, the motor strands autonomously walked along the track, leading to the release of many fluorescent molecules. Gold nanorods (AuNRs) with tunable aspect ratio-dependent plasmonic extinction band can also be utilized to quench the luminescence. For instance, Chen’s group reported a simple paper-supported biosensor with AuNRs to quench

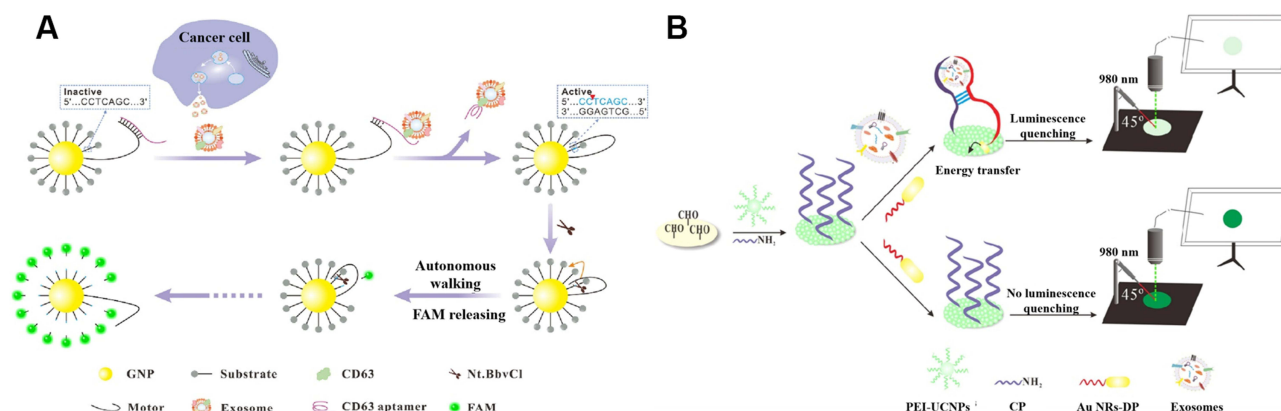


Figure 3 (A) Schematic of the exosome-triggered enzyme-powered DNA motors for exosome detection. Reprinted with permission from Yu Y, Zhang WS, Guo Y, Peng H, Zhu M, Miao D, Su G. Engineering of exosome-triggered enzyme-powered DNA motors for highly sensitive fluorescence detection of tumor-derived exosomes. *Biosens Bioelectron.* 2020;167:112482–112490. Copyright 2020 Elsevier B.V.⁹⁹ (B) Schematic of paper-supported aptasensor based on the LRET between UCNPs and AuNRs for the determination of exosomes. Reprinted with permission from Chen X, Lan J, Liu Y, et al. A paper-supported aptasensor based on upconversion luminescence resonance energy transfer for the accessible determination of exosomes. *Biosens Bioelectron.* 2018;102:582–588. Copyright 2018 Elsevier B.V.¹⁰⁰

the luminescence of upconversion nanoparticles (UCNPs) through luminescence resonance energy transfer (LRET).¹⁰⁰ As illustrated in Figure 3B, the sequence of aptamer toward CD63 protein is divided into two flexible ssDNA pieces with different sequence (CP and DP). Branched polyethylenimine (PEI)-modified UCNPs and CP were immobilized on the surface of filter paper by the formation of Schiff base. When exosomes were added, CD63 on the surface of exosomes facilitated the combination of DP and CP together into the intact aptamer tertiary, resulting in the close of AuNRs and UCNPs. The distance between AuNRs and UCNPs was shortened to allow for the occurrence of LRET. However, with the CD63, there was no interaction between two fragments and the LRET could not occur.

Graphene oxide (GO) can interact with DNA or RNA through π - π stacking interactions and thus quench the fluorescence of dye-labeled DNA/RNA probe through FRET. It is a fascinating nanomaterial to develop DNA-based “signal on/off” fluorescent biosensors for exosome detection.¹⁰¹ Wang et al designed a DNase I enzyme-aided signal amplification strategy for fluorescence analysis of colorectal cancer (CRC) exosomes based on the interaction between GO and aptamer.¹⁰² As illustrated in Figure 4A, the fluorescence of two aptamers (CD63 and epithelial cell adhesion molecule or EpCAM) labeled with different fluorophores was quenched by GO. In the presence of exosomes, two aptamers were bound to the target proteins of CD63 and EpCAM on the surface of CRC exosomes and then released from the surface of GO. DNase I promoted the digestion of the aptamers and induced the release of exosomes to

liberate more aptamers, thus achieving a signal amplification. Few exosomes resulted in the release of numerous dyes and the restoration of fluorescence. Li et al developed a homogeneous magneto-fluorescent nanosensor for exosome analysis using GO as the quencher to reduce the background signal.¹⁰³ As shown in Figure 4B, after exosomes were isolated by GPC-1 antibody-coated MBs, an extended CD63 aptamer was used to label the exosomes and the extended terminus served as a toehold to initiate the strand displacement, resulting in the formation of a large number of DNA three-way junctions (TWJ). After the magnetic separation, DNA TWJ in the supernatant could adsorb numerous positively charged derivatives of tetraphenylethene (TPE) aggregation-induced emission luminogens (AIEgens) through the electrostatic interaction. As a result, an enhanced fluorescence signal was observed. Meanwhile, GO was added to quench the fluorescence of AIEgens-stained ssDNA. The novel method achieved a wide linear detection range and the detection limit was calculated to be 6.56×10^4 particles/ μ L. In addition, MoS₂-multiwall carbon nanotubes nanocomposites were employed to quench the fluorescence of dye-labeled CD63 antibody, which could be restored after the immunoreaction between exosome and antibody.¹⁰⁴

As one subclass of 2D transition-metal carbides and carbonitrides materials, ultrathin MXenes have attracted much attention in biomedical applications due to their superior properties similar to those of GO. Based on their outstanding quenching efficiency, MXenes have been intensively utilized to construct fluorescent biosensors for the detection of targets, including DNA, RNA and

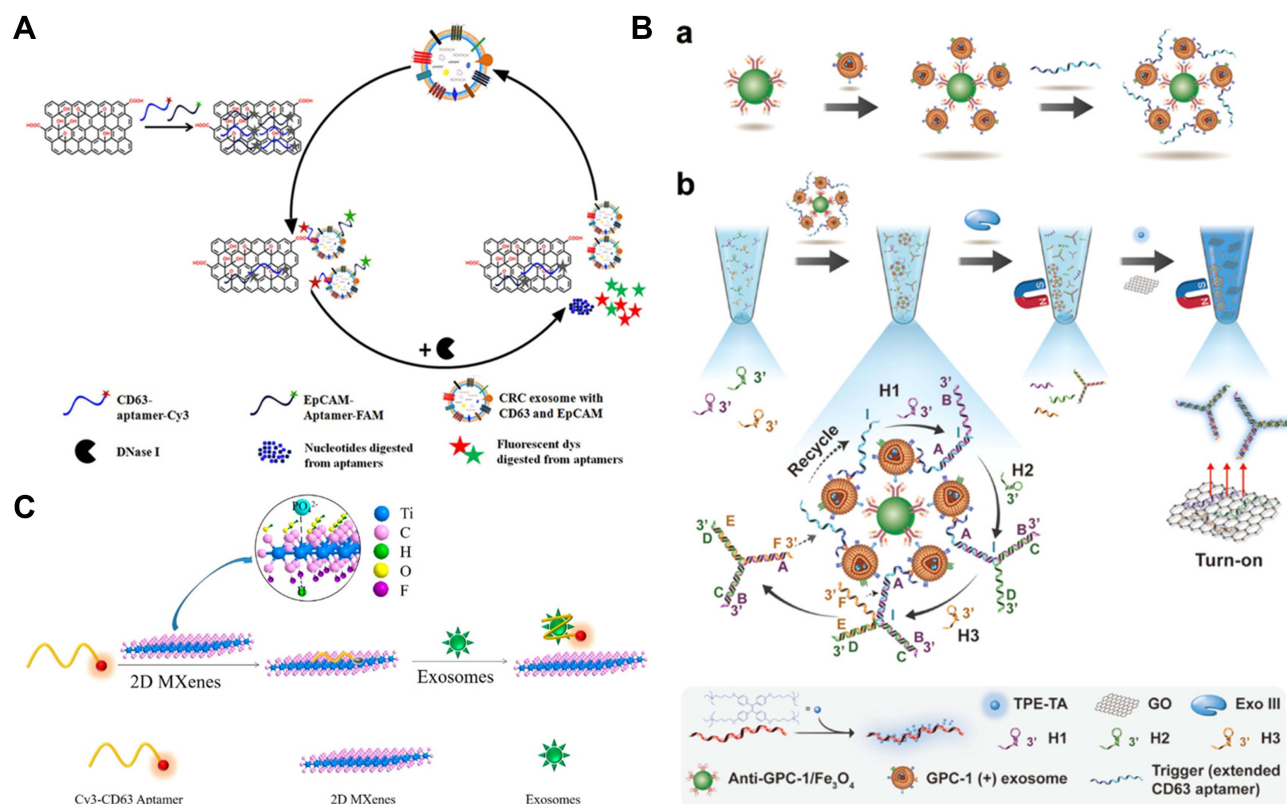


Figure 4 (A) Schematic of enzyme-aided fluorescence amplification based on GO-DNA aptamer interactions for exosome detection. Reprinted with permission from Wang H, Chen H, Huang Z, Li T, Deng A, Kong J. DNase I enzyme-aided fluorescence signal amplification based on graphene oxide-DNA aptamer interactions for colorectal cancer exosome detection. *Talanta*. 2018;184:219–226. Copyright 2018 Elsevier B.V.¹⁰² (B) Schematic of homogeneous magneto-fluorescent nanosensor for tumor-derived exosome isolation and analysis. (a) Tumor-derived exosomes are specifically captured by GPC-1 antibody coated magnetic beads and subsequently bind with extended CD63 aptamers, forming a bead–exosome–aptamer complexes. (b) Captured exosomes are detected in a homogeneous solution by aptamer-triggered DNA TWJs cyclic assembly strategy along with TPE-TA and the GO-based “turn-on” fluorescent system. Reprinted with permission from Li B, Pan W, Liu C, et al. Homogenous magneto-fluorescent nanosensor for tumor-derived exosome isolation and analysis. *ACS Sens*. 2020;5:2052–2060. Copyright 2020 American Chemical Society.¹⁰³ (C) Schematic of Cy3-CD63 aptamer was mixed with MXenes aqueous solution and then added exosomes. Reprinted with permission from Zhang Q, Wang F, Zhang H, Zhang Y, Liu M, Liu Y. Universal Ti3C2 MXenes based self-standard ratiometric fluorescence resonance energy transfer platform for highly sensitive detection of exosomes. *Anal Chem*. 2018;90:12737–12744. Copyright 2018 American Chemical Society.¹⁰⁵

proteins. Recently, Liu and co-workers reported a Ti₃C₂ MXenes-based self-standard ratiometric FRET platform for the detection of exosomes (Figure 4C).¹⁰⁵ In the work, Cy3-labeled CD63 (Cy3-CD63) aptamers were adsorbed on the surface of MXenes by hydrogen-bond and metal-chelate interactions. The fluorescence of Cy3-CD63 aptamer was quenched by FRET and the intrinsic fluorescence of MXenes showed little change as a standard reference. Exosomes could specifically bind to the aptamers and induce their release from the surface of MXenes, thus leading to the recovery of fluorescence signal.

Colorimetric Biosensors

Colorimetric biosensors have attracted extensive attention because of their low cost and convenient readout. The results can be quickly observed with naked eyes. Thus, colorimetric assay is of great importance for point-of-care

testing in facility-limited settings. Normally, enzymes are required to catalyze the chromogenic reaction in colorimetric assays.^{106,107} In traditional ELISA for the detection of exosomes, horseradish peroxidase (HRP) linked with detection antibody was always used to catalyze the reaction between H₂O₂ and colorimetric substrate 3,3',5,5'-tetramethylbenzidine (TMB).^{108,109} Then, the color of solution changes from colorless to blue. However, they face the problems of low reproducibility and sensitivity (with a minimum amount of 3 µg of purified samples).¹¹⁰ Hemin/G-quadruplex with HRP-mimicking catalytic activity has also been widely used in bioassays for signal amplification.^{111,112} To improve the sensitivity, several strategies have been proposed for signal amplification, such as using immune-magnetic nanoparticles (MNPs) to enrich exosomes and using NPs to enhance the amount of enzymes for signal output.^{113–115} For example, He et al

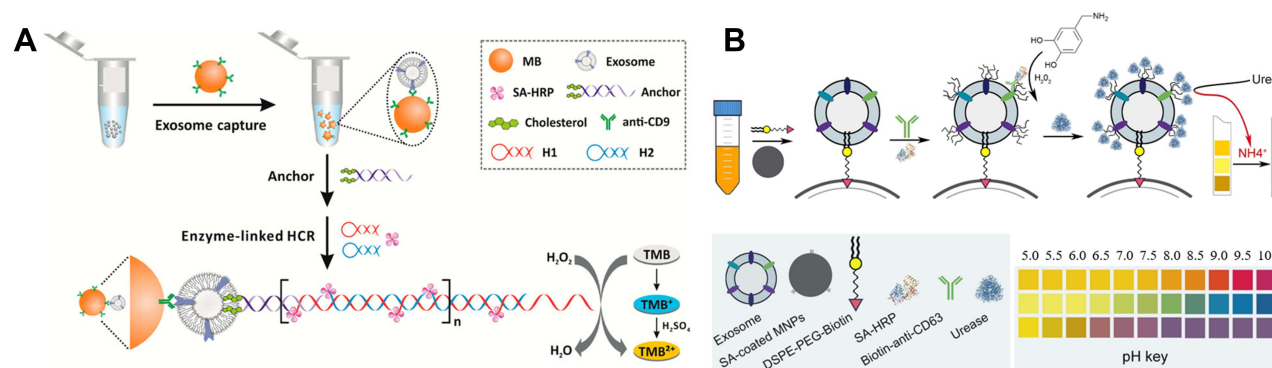


Figure 5 (A) Schematic of the colorimetric method for exosome detection by a combination of immunoaffinity separation and cholesterol-based signal amplification. Reprinted with permission from He F, Liu H, Guo X, Yin BC, Ye BC. Direct exosome quantification via bivalent-cholesterol-labeled DNA anchor for signal amplification. *Anal Chem.* 2017;89:12968–12975. Copyright 2017 American Chemical Society.¹¹⁶ **(B)** Schematic of magnetic capture of exosomes, HRP-mediated PDA engineering of exosomes and urease immobilization for point-of-care testing. Reprinted with permission from Yang Y, Li C, Shi H, Chen T, Wang Z, Li G. A pH-responsive bioassay for paper-based diagnosis of exosomes via mussel-inspired surface chemistry. *Talanta.* 2019;192:325–330. Copyright 2019 Elsevier B.V.¹¹⁸

reported the direct quantification of exosomes based on HCR- and HRP-mediated signal amplification.¹¹⁶ As shown in Figure 5A, after exosomes were captured by CD9 antibody-coated MBs, the bivalent-cholesterol-labeled DNA probes were added to recognize the lipid membrane of exosomes via the hydrophobic cholesterol moiety. The DNA probe triggered the HCR and then numerous SA-HRP conjugates were captured by the DNA polymer for catalyzing the chromogenic reaction. The proposed assay showed a detection limit of 2.2×10^3 particles/ μ L. In addition, DNA nanoflowers were also employed to encapsulate HRP, thus improving the loading number of enzyme in signal output.¹¹⁷ Yang et al proposed a pH-responsive paper-based bioassay for the detection of exosomes.¹¹⁸ As shown in Figure 5B, after the SA-coated MNPs-based capture of exosomes, HRP conjugated with CD63 antibody catalyzed the formation of polydopamine film on the exosome surface, thus allowing for the binding of ureases.¹¹⁹ The captured ureases could hydrolyze urea into ammonia and carbon dioxide, resulting in the change of solution pH value from 5 to 10 and the color change of commercially available pH test paper. However, the utilization of natural enzyme is confronted of severe disadvantages of low stability, high-cost and complicated preparation process.

Au and Ag NPs with local surface plasmon resonance (LSPR) characteristics exhibit higher extinction coefficient than the organic chromogens. Such NPs have been widely used as the alternative substrates to develop plasmonic colorimetric methods for bioassays. The detection principles of NPs-based colorimetric strategies can be divided into two subclasses: aggregation/disaggregation and etching/growth.

Typically, Maiolo et al presented a simple plasmonic colorimetric strategy for the determination of exosomes.¹²⁰ As shown in Figure 6A, AuNPs could aggregate at the lipid membrane of exosomes, resulting in the shift and broaden of LSPR absorption spectrum and the change of solution color from red to blue. However, in the presence of exosome and protein contaminants, the formation of protein corona around AuNPs prevented the aggregation, and the LSPR absorption kept unchanged. Tan and co-workers developed a colorimetric aptasensor for profiling of exosomal proteins (Figure 6B).¹²¹ In this work, conjugation of aptamer with AuNPs prevented NPs from aggregation in high salt solution. However, the specific interaction between aptamer and exosome made aptamer leave the surface of AuNPs and resulted in the aggregation of AuNPs with the color change from red to blue. Liu et al reported a rapid and convenient colorimetric method for the detection of exosomes at ultralow concentrations by integrating target-induced proximity ligation assay (PLA) with recombinase polymerase amplification (RPA) and transcription-mediated amplification (TMA).¹²² As illustrated in Figure 6C, after two PLA probes bound to the protein LMP1 on the surface of exosomes, two DNA probes hybridized with each other. Under the RPA and TMA amplification, multiple copies of RNA transcripts were generated, which could induce the aggregation of the DNA-modified AuNPs and the change of solution color. Furthermore, the principle of AuNPs-based color assay have been introduced into LFA for rapid and sensitive analysis of exosomes.^{123–126} In addition, because AuNR is more sensitive to the change of local media environment, and the AuNR-based color change is more realistic, AuNR-based colorimetric assays exhibit better

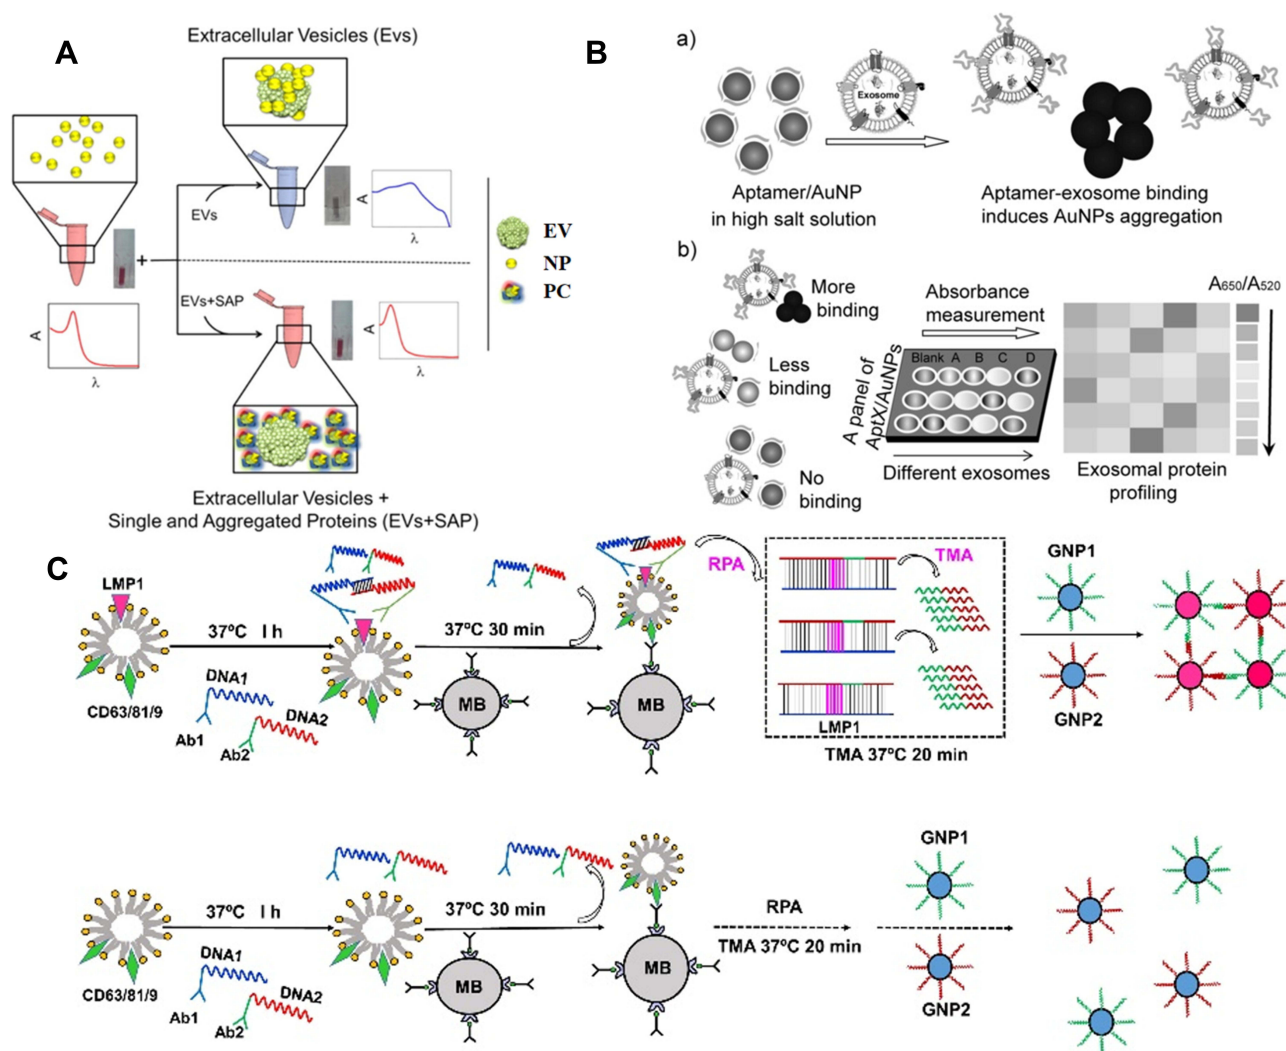


Figure 6 (A) Schematic of nanoplasmic assay for probing by eye protein contaminants (single and aggregated exogenous proteins, SAP) in EV preparations. Reprinted with permission from Maiolo D, Paolini L, Di Noto G, et al. Colorimetric nanoplasmic assay to determine purity and titrate extracellular vesicles. *Anal Chem.* 2015;87:4168–4176. Copyright 2015 American Chemical Society.¹²⁰ (B) Schematic of the aptamer/AuNP complex for molecular profiling of exosomal proteins. (a) Schematic of the displacement of aptamers from gold nanoparticles by binding with exosome surface protein and the concomitant aggregation of gold nanoparticles. (b) Profiling of different exosome surface proteins with the aptamer/AuNP complex. Reprinted with permission from Jiang Y, Shi M, Liu Y, et al. Aptamer/AuNP biosensor for colorimetric profiling of exosomal proteins. *Angew Chem.* 2017;129:12078–12082. Copyright 2017 Wiley-VCH.¹²¹ (C) Schematic of the PLA-RPA-TMA assay. Reprinted with permission from Liu W, Li J, Wu Y, et al. Target-induced proximity ligation triggers recombinase polymerase amplification and transcription-mediated amplification to detect tumor-derived exosomes in nasopharyngeal carcinoma with high sensitivity. *Biosens Bioelectron.* 2018;102:204–210. Copyright 2018 Elsevier B.V.¹²²

performances. Zhang et al reported the multicolor visual assay of exosome by the enzyme-catalyzed metallization of AuNR and HCR amplification.¹²⁷ As depicted in Figure 7A, after exosomes were captured and labeled with cholesterol-modified DNA probes, the terminal DNA probes initiated the HCR assembly. Large numbers of alkaline phosphatase (ALP) molecules were loaded on the exosome surface to catalyze the production of ascorbic acid (AA) and the in-situ formation of silver shells on AuNRs, alongside with a vivid change of solution color. Moreover, Au nanobipyramid@MnO₂ nanosheet was also used as the substrate for colorimetric detection of exosomes.¹²⁸

During the exosome-induced competitive reaction, a large amount of ALP molecules were released into the solution by few exosomes and the free ALP catalyzed the generation of AA to etch Au nanobipyramid@MnO₂ nanosheet, accompanied with multicolor change.

Since Fe₃O₄NPs were reported to show peroxidase-like activity, more and more nanomaterials called nanozymes have proven to show catalytic ability and have been integrated into colorimetric bioassays.¹²⁹ Compared to the natural enzymes, the nanozymes show attractive advantages of improved stability, low cost and ease of storage. Surface charge and composition are two crucial roles to

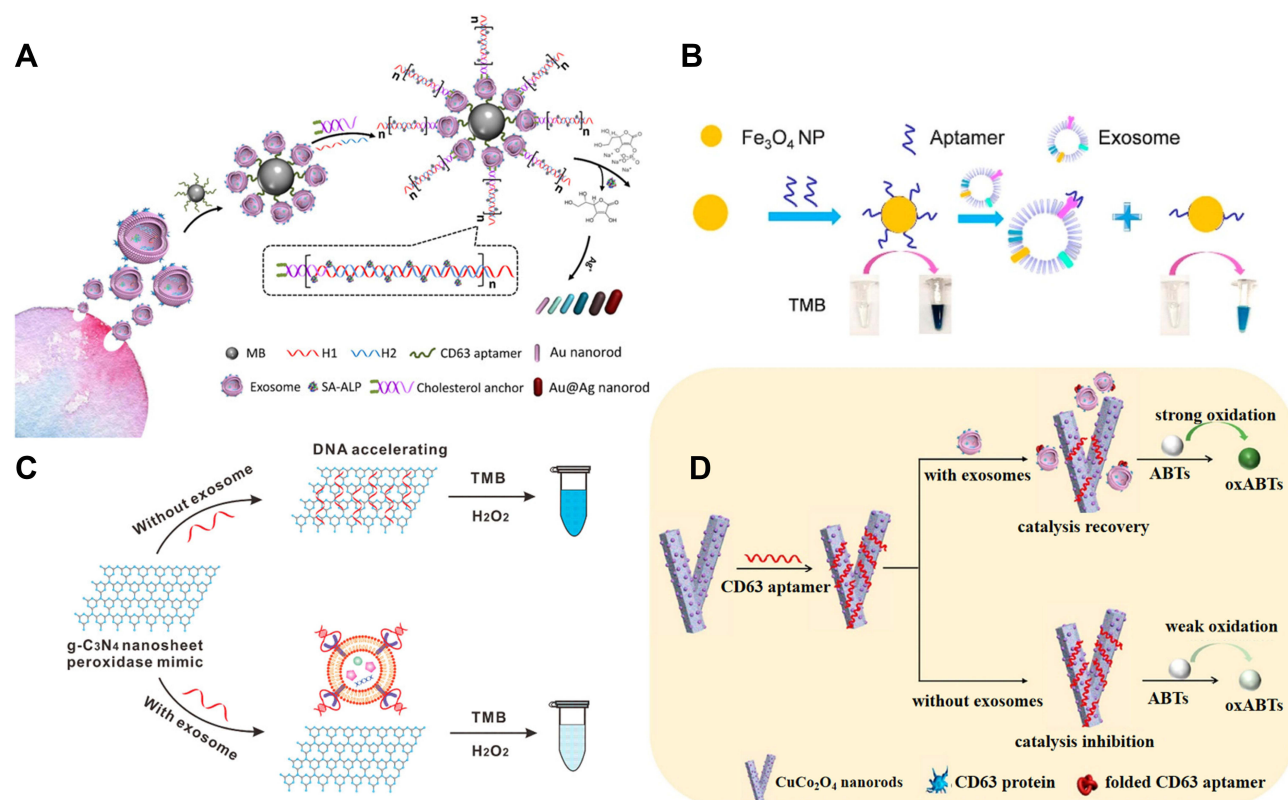


Figure 7 (A) Schematic of the mechanism for multicolor visual detection of exosomes based on HCR and enzyme-catalyzed metallization of Au NRs. Reprinted with permission from Zhang Y, Wang D, Yue S, et al. Sensitive multicolor visual detection of exosomes via dual signal amplification strategy of enzyme-catalyzed metallization of Au nanorods and hybridization chain reaction. *ACS Sens.* 2019;4:3210–3218. Copyright 2019 American Chemical Society.¹²⁷ (B) Schematic of the visible detection of exosomes based on ssDNA-enhanced Fe_3O_4 NPs nanozyme activity. Reprinted with permission from Chen J, Xu Y, Lu Y, Xing W. Isolation and visible detection of tumor-derived exosomes from plasma. *Anal Chem.* 2018;90:14207–14215. Copyright 2018 American Chemical Society.¹³¹ (C) Schematic of DNA aptamer accelerating the intrinsic peroxidase-like activity of g- C_3N_4 NSs for the detection of exosomes. Reprinted with permission from Wang YM, Liu JW, Adkins GB, et al. Enhancement of the intrinsic peroxidase-like activity of graphitic carbon nitride nanosheets by ssDNAs and its application for detection of exosomes. *Anal Chem.* 2017;89:12327–12333. Copyright 2017 American Chemical Society.¹³² (D) Schematic of the detection mechanism for the visible detection of exosomes based on ssDNA-enhanced Fe_3O_4 NPs nanozyme activity. Reprinted with permission from Zhang Y, Su Q, Song D, Fan J, Xu Z. Label-free detection of exosomes based on ssDNA-modulated oxidase-mimicking activity of CuCo_2O_4 nanorods. *Anal Chim Acta.* 2021;1145:9–16. Copyright 2021 Elsevier B.V.¹³⁴

regulate the catalytic activity of nanozymes. ssDNA can improve the peroxidase-mimicking activity of nanozymes.¹³⁰ Chen et al reported the colorimetric assay of exosomes through ssDNA aptamer-enhanced peroxidase activity of Fe_3O_4 NPs (Figure 7B).¹³¹ They found that aptamers attached on the surface of Fe_3O_4 NPs could increase the affinity between NPs and TMB, thus leading to the enhancement of peroxidase activity. In the work, anion exchange method was first designed to extract exosomes from plasma. Then, the captured exosomes bound to aptamers from NPs and led to the decrease in the catalytic activity. Moreover, Wang et al developed the ssDNA-enhanced nanozyme-based colorimetric method for exosome detection (Figure 7C).¹³² They demonstrated that ssDNA could accelerate the intrinsic peroxidase-mimicking activity of graphitic carbon nitride nanosheets (g- C_3N_4 NSs) through the electrostatic and aromatic

stacking interactions between ssDNA and TMB. However, CD63 on the surface of exosomes could competitively bind with ssDNA aptamer and reduce the enhancement of the peroxidase-mimicking activity. The method is sensitive and could determine exosomes in the range from 1.9×10^6 to 3.38×10^7 particles/ μL . Xia et al employed ssDNA-modified single-wall carbon nanotubes for the detection of exosomes by the same principle.¹³³ On the contrary, Zhang et al reported the label-free colorimetric assay of exosomes based on ssDNA-inhibited oxidase-like activity of CuCo_2O_4 nanorods (NRs).¹³⁴ As shown in Figure 7D, CuCo_2O_4 NRs could catalyze the oxidation of ABTS with O_2 as the electron acceptor, instead of volatile H_2O_2 . The negatively charged CD63 aptamers were adsorbed on the CuCo_2O_4 NRs through the electrostatic interaction and the oxidase-like activity of NRs was inhibited by hindering the electron transfer between NRs and

substrates. However, in the presence of exosomes, aptamers were released from the CuCo_2O_4 NRs and the oxidase-like activity was restored.

Surface Plasmon Resonance Biosensors

Surface plasmon resonance (SPR) is a label-free, real-time sensing technique to study and quantify biomolecular interaction.¹³⁵ It can monitor the change of refractive index in close proximity to the gold surface (within 200 nm), resulting from binding event-induced increase of thickness. Moreover, it possesses the merits of high signal-to-noise, good compatibility with microfluidic technique and advanced surface modifications. Therefore, exosomes with around 100 nm size and large mass can be detected by SPR, whose size fits within the surface plasmon wave depth. To date, a series of label-free SPR

biosensors for exosome detection have been developed by modifying the sensor surface with antibodies specific to the membrane proteins on exosome.^{136–145} To overcome the slow diffusion-limited mass transfer, magnetic nanoparticles can be utilized to pre-concentrate exosomes on the sensor surface under an external magnetic field gradient.¹⁴⁶ However, the poor sensitivity of the methods limits their further applications for analyzing trace targets in complex samples.

AuNPs can enhance the SPR signal through plasmonic coupling.^{147–150} Wang et al proposed a SPR aptasensor for quantification of cancerous exosomes with dual AuNPs-assisted signal amplification.¹⁵¹ As illustrated in Figure 8, the gold chip was functionalized with aptamers to capture exosomes. Aptamer/ T_{30} -modified AuNPs were further used to label exosomes on the Au film. The sensitivity of

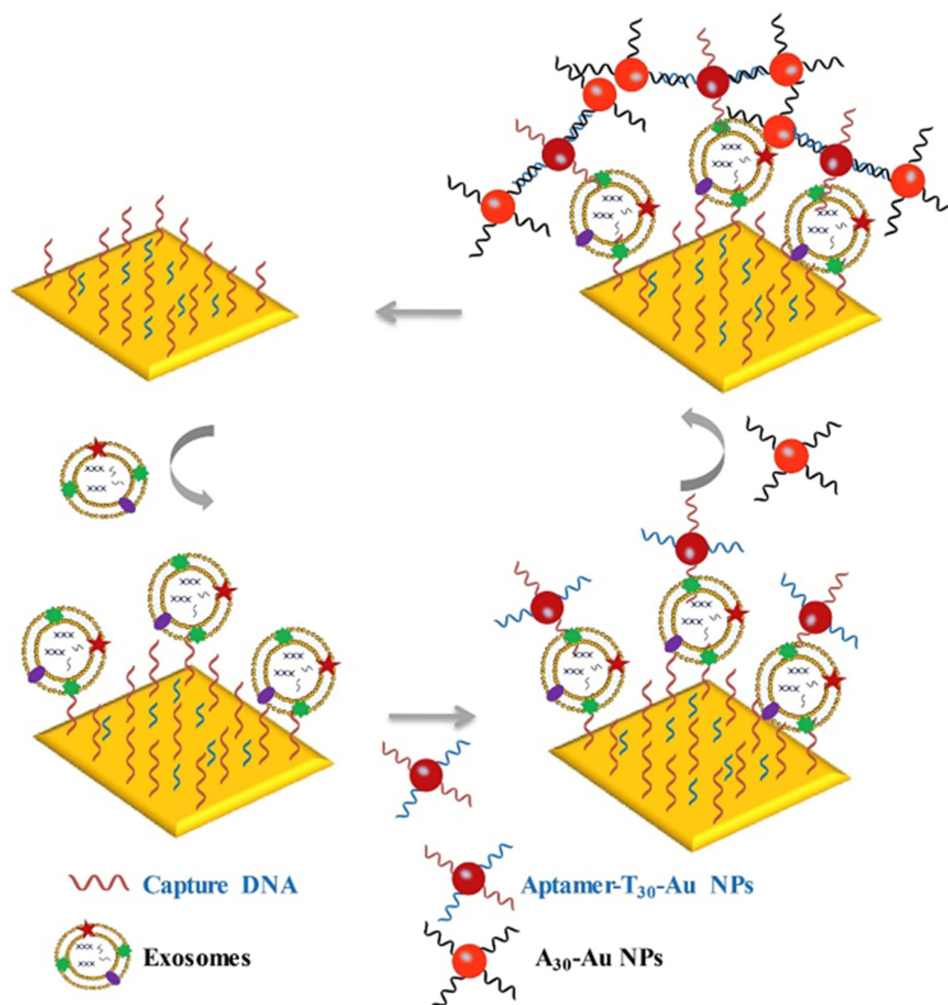


Figure 8 Schematic of dual AuNP-assisted signal amplification for SPR determination of exosomes. Reprinted with permission from Wang Q, Zou L, Yang X, et al. Direct quantification of cancerous exosomes via surface plasmon resonance with dual gold nanoparticle-assisted signal amplification. *Biosens Bioelectron.* 2019;135:129–136. Copyright 2019 Elsevier B.V.¹⁵¹

the biosensor is very high because of the electronic coupling between the gold film and AuNPs. For increasing the specificity, they further developed a dual-aptamers-based SPR strategy for the determination of human hepatic carcinoma (SMMC-7721) exosomes.¹⁵² In addition, combining with DNA-based signal amplification, Ding's group reported a hydrogel-AuNP supramolecular sphere (H-Au)-based SPR biosensor for analysis of prostate cancer-derived exosomes.¹⁵³ The H-Au network was prepared via the self-assembly of DNA chains and DNA-modified AuNPs. The PSMA-specific aptamer-functionalized MBs were used to transduce target exosomes into triple DNAs, which could initiate the terminal transferase-catalyzed generation of polyA tails than can bind to the H-Au network on the SPR surface. This biosensor had a wide linear range from 1.00×10^2 to 1.00×10^4 particles/ μL .

Surface Enhanced Raman Scattering Biosensors

Raman spectroscopy can provide a characteristic fingerprint spectrum. However, the signal intensity is always too weak to be distinguished. Since SERS effect was discovered, a significant interest in SERS study was aroused. Generally, metal nanostructures or nanomaterials can be employed to amplify the signal through chemical and electromagnetic field enhancement. SERS spectroscopy has been used for the design of biosensors by label-free analysis and SERS-tag-based methods.¹⁵⁴

Label-free SERS analysis is mainly based on the use of roughened or nanosized SERS substrate to enhance the weak Raman vibration signal of exosomal biomolecules with fingerprint characters. For example, Avella-Oliver et al reported the label-free SERS analysis of exosomes with large-scale substrates from recordable compact disk by coating it with silver.¹⁵⁵ This cost-effective technology provided an alternative solution to perform SERS bioassays in non-specialized environments. Inspired by the concept of beehives, Dong et al suggested that the Au-coated TiO_2 macroporous inverse opal (MIO) structures could be used as the SERS substrates for label-free detection of exosomes.¹⁵⁶ As shown in Figure 9A, different from traditional SERS substrates, the MIO structure could capture exosomes by its interconnected nanoscale pore networks, exhibiting a prominent "slow light effect" and enhancing the Raman signal of exosomes by the SERS effect of Au layer. The SERS intensity of 1087 cm^{-1} from the P-O bond within phosphoproteins on the surface of

exosomes was used as the detection criterion. Because of the heterogeneity, the Raman spectra of exosomes show complex and inconsistent data, which are difficult to be classified. For this view, principal component analysis was employed to monitor the Raman signal, and a meaningful pattern for exosome analysis was obtained.^{157–159}

Au and Ag nanomaterials with LSPR have been utilized as the SERS-active nanotags to enhance the signal intensity of Raman dyes. With immunomagnetic beads and for the capture of exosomes, several aptamer or antibody-modified SERS nanotags have been developed for exosome detection via the formation of antibody-exosome-aptamer sandwich-type immunocomplexes.^{160–163} Microfluidic Raman biochips were also fabricated to isolate and determine exosomes in situ.⁴³ Typically, Wang's group reported an effective approach for the detection of exosomes by simultaneously profiling multiple protein biomarkers on the surface.¹⁶⁴ As shown in Figure 9B, three specific nanotags for antibody modification were prepared and labeled in the filtered conditional exosome-suspension medium. Then, the antibody-modified CD63-conjugated MBs were added for the sandwich-like immunoassays. The heterogeneous antigens expressed on diverse exosomes limited the applications of the methods based on the antigen-antibody/aptamer interaction. Liu's group proposed a general, facile, and robust strategy to label exosomes with maleimide (Mal) tags by the hydrophobic insertion.¹⁶⁵ As shown in Figure 9C, maleimide-terminated DSPE-PEG (DSPE-PEG-Mal) as labeling probe was inserted into the lipid membranes. Mal group could be conjugated with the thiol-containing species (1,6-hexanedithiol) via the click chemistry and further bound to bare AuNPs for SERS analysis. Wang's group developed a SERS biosensor for multiple assays of exosomes with gold layer-coated MBs as SERS probes which were modified with three different types of Raman reporters and aptamers.¹⁶⁶ Besides, Kwizera et al presented a method for exosome detection by using cationic AuNRs as SERS tags to label exosomes through the electrostatic attraction.¹⁶⁷ The "hot spots" generated in the AuNP-AuNP junctions due to the plasmon coupling effect can intensify the Raman signal of SERS molecules. For this view, Ning et al reported the multiple SERS assays of exosomes using gold-silver bimetallic nanotrepangs, in which different Raman reporter molecules were confined in the interfaces of gold core and silver shell.¹⁶⁸ Zhang et al designed a novel Raman probe for the assays of exosomes by assembling AuNPs in triangular pyramid DNA (TP-DNA).¹⁶⁹ As illustrated in Figure 9D, TP-DNA was

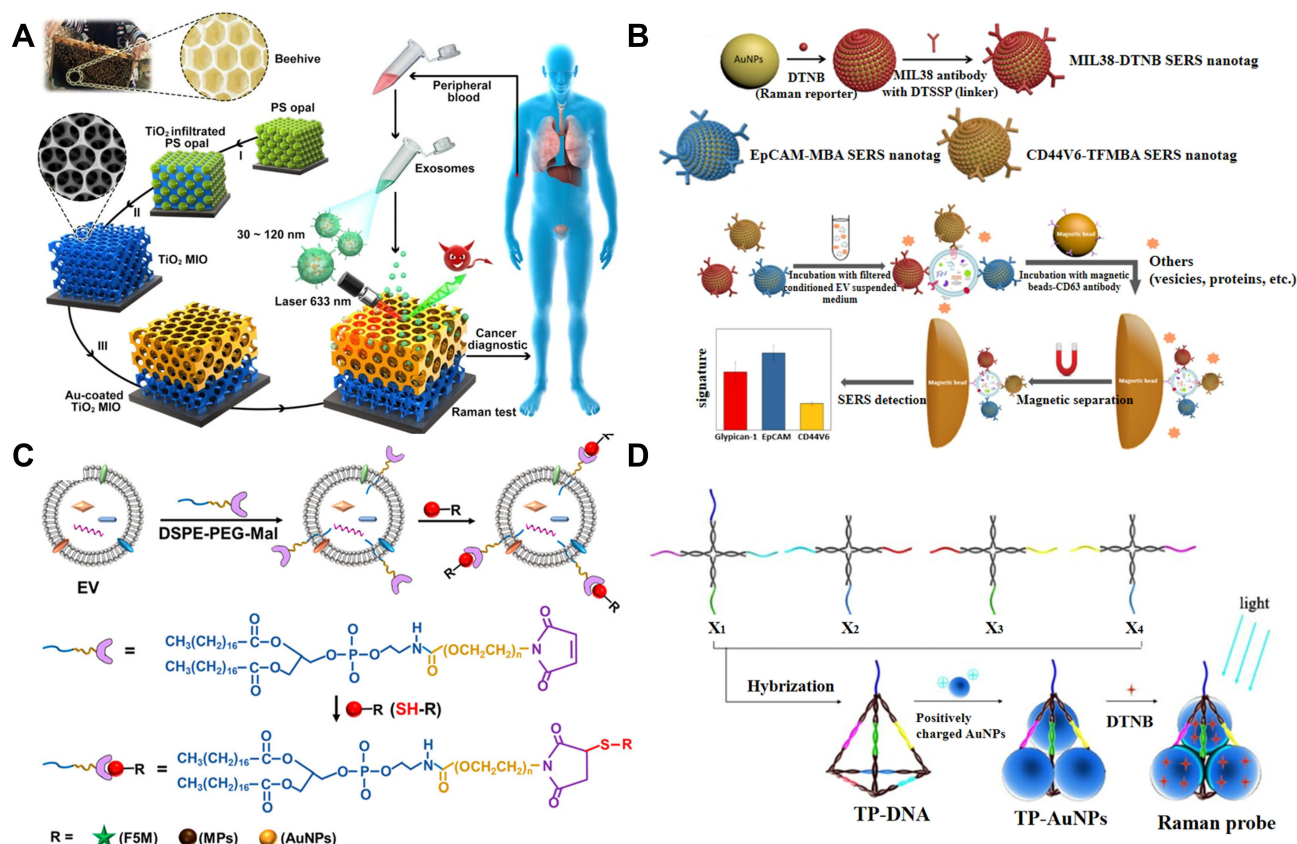


Figure 9 (A) Schematic representation of detection process and design inspiration of the Au-coated TiO₂ MIO SERS probe. Reprinted with permission from Dong S, Wang Y, Liu Z, et al. Beehive-inspired macroporous SERS probe for cancer detection through capturing and analyzing exosomes in plasma. *ACS Appl Mater Interfaces*. 2020;12:5136–5146. Copyright 2020 American Chemical Society.¹⁵⁶ (B) Schematic representation of preparation of three types of SERS nanotags and molecular phenotype profiling of exosomes using SERS nanotags and CD63 antibody-functionalized MBs. Reprinted with permission from Zhang W, Jiang L, Diefenbach RJ, et al. Enabling sensitive phenotypic profiling of cancer-derived small extracellular vesicles using surface-enhanced Raman spectroscopy nanotags. *ACS Sens*. 2020;5:764–771. Copyright 2020 American Chemical Society.¹⁶⁴ (C) Schematic of exosomes engineering based on a hydrophobic insertion strategy with DSPE-PEG-Mal. Reprinted with permission from Di H, Zeng E, Zhang P, et al. General approach to engineering extracellular vesicles for biomedical analysis. *Anal Chem*. 2019;91:12752–12759. Copyright 2019 American Chemical Society.¹⁶⁵ (D) Schematic representation of assembling AuNPs in triangular pyramid DNA. Reprinted with permission from Zhang X, Liu C, Pei Y, Song W, Zhang S. Preparation of a novel Raman probe and its application in the detection of circulating tumor cells and exosomes. *ACS Appl Mater Interfaces*. 2019;11:28671–28680. Copyright 2019 American Chemical Society.¹⁶⁹

prepared through the hybridization of four X-shaped DNA sequences and then the positively charged AuNPs and Raman reporter molecules were entrapped through the electrostatic interactions. Besides, laser-tweezers Raman spectroscopy has also been employed to determine exosomes with individual nanoparticle for signal enhancement.¹⁷⁰

Nanomaterials-Based Electrochemical Biosensors for Exosome Detection

Electrochemical Biosensors

Electrochemical biosensor has been recognized as an excellent platform for biological sample analysis due to its advantages of high sensitivity, low cost, rapid response and low sample volume.^{171,172} Several classic

electrochemical techniques are frequently utilized in bioassays, including amperometry, voltammetry, impedimetry and field effect transistor. Nanomaterials mainly play two vital roles in these techniques: as the electrode substrate to improve the electron transfer and as the functional nanotags for signal amplification.¹⁷³

Direct Detection

Direct electrochemical detection is achieved by monitoring the change of electrical conductivity of electrode by the target-induced electrical signal change.^{174–177} The method can quantify exosomes without labeling step, thus shortening the response time. For example, Tan and co-workers presented an electrochemical aptasensor for direct determination of cancerous exosomes by using DNA nanotetrahedra to immobilize aptamer on the electrode surface to improve

the accessibility of exosomes.¹⁷⁸ Davis's group reported an immunosensor for the analysis of exosomes by electrochemical impedance spectroscopy.¹⁷⁹ Vaidyanathan developed a multiplexed device to detect exosomes by alternating current electrohydrodynamic induced nanoshearing.¹⁸⁰

AuNPs with good electrical conductivity and easy of functionalization have been widely utilized to modify the sensor electrode. Cucurbit[7]uril with excellent supramolecular recognition ability toward ferrocene (Fc) has been widely used as the receptor in electrochemical analysis. Liu et al reported a label-free electrochemical aptasensor for exosome detection based on the host-guest interaction between cucurbit[7]uril and Fc.¹⁸¹ As illustrated in Figure 10A, cucurbit[7]uril was immobilized on the AuNPs-modified electrode for the capture of Fc-labeled CD63 aptamer. The aptamer bound to the target exosome with high affinity can be released from the electrode surface, thus resulting in the decrease of electrochemical signal. Sun et al developed a dual-signal and intrinsic self-calibration aptasensor for direct detection of exosomes.¹⁸² As shown in Figure 10B, ITO slice was modified with Fc-doped metal-organic frameworks (ZIF-67) by electrodeposition and black phosphorus nanosheets (BPNSs). Then, the methylene blue-labeled ssDNA aptamers were adsorbed on the electrode surface. The platform exhibited dual redox-signal responses from methylene blue and Fc. In the presence of exosomes, the aptamers were desorbed from the electrode surface, leading to the decrease of redox current of methylene blue. In this process, no significant change was observed for the current of

Fc. The intrinsic self-calibration aptasensor showed a detection limit down to 0.1 particles/ μ L.

Field effect transistor (FET) biosensor is a promising label-free detection tool, which can monitor the microelectrical signal caused by the interaction between target and recognition element on the sensing interface.¹⁸³ Yu et al designed a reduced graphene oxide (rGO)-based FET biosensor for electrical and label-free quantification of exosomes.¹⁸⁴ In this paper, 1-pyrenebutanoic acid succinimidyl ester was modified on the rGO surface through the π - π stacking interaction between pyrene and graphene. Then, CD63 antibody was covalently immobilized on the FET surface. The net carrier density changed with the introduction of negatively charged exosomes, thus leading to the left shift of the Dirac point.

Sandwich-Like Methods

Although the label-free electrochemical method is simple, it shows poor sensitivity and selectivity. Therefore, different types of sandwich-like methods were developed for bioassays. Generally, the electrode was modified with a biorecognition element to capture exosome, and the another biorecognition element modified with a signal reporter was added to recognize the captured exosome and produce an electrical signal. Enzymes and electroactive molecules are usually used as the signal reporters for signal amplification.¹⁸⁵ For example, Doldan et al reported an electrochemical immunosensor for the determination of exosomes using HRP-conjugated antibody.¹⁸⁶ An et al designed an electrochemical aptasensor for the detection of tumor exosomes by the HCR assembly to linking numerous HRP molecules for catalytic redox

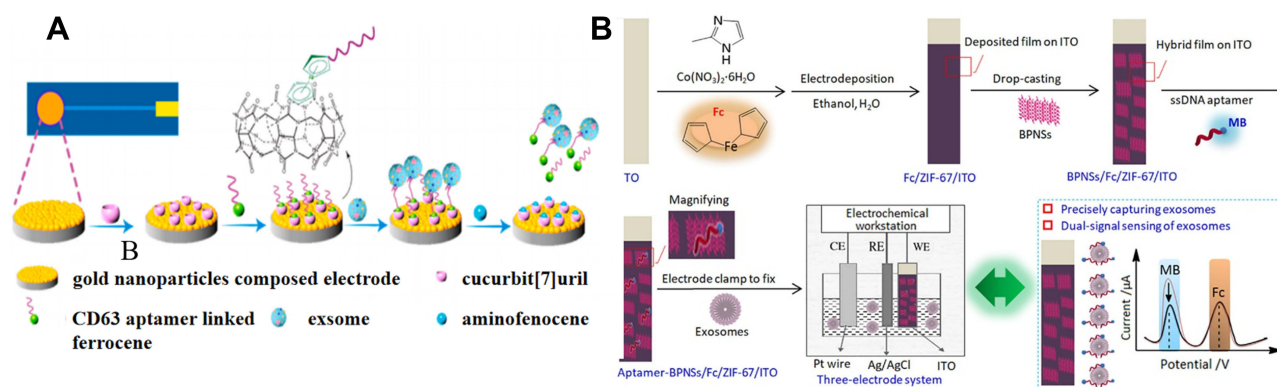


Figure 10 (A) Schematic representation of the electrochemical aptasensor for exosomes capture and release based on specific host-guest interactions between cucurbit[7]uril and Fc. Reprinted with permission from Liu Q, Yue X, Li Y, et al. A novel electrochemical aptasensor for exosomes determination and release based on specific host-guest interactions between cucurbit [7]uril and ferrocene. *Talanta*. 2021;232:122451–122458. Copyright 2021 Elsevier B.V.¹⁸¹ **(B)** Schematic representation of the construction process and application of a dual-signal and intrinsic self-calibration aptasensor of exosomes based on a functional hybrid thin-film sensing platform aptamer-BPNSs/Fc/ZIF-67/ITO. Reprinted with permission from Sun Y, Jin H, Jiang X, Gui R. Assembly of black phosphorus nanosheets and MOF to form functional hybrid thin-film for precise protein capture, dual-signal and intrinsic self-calibration sensing of specific cancer-derived exosomes. *Anal Chem*. 2020;92:2866–2875. Copyright 2020 American Chemical Society.¹⁸²

reactions.¹⁸⁷ He and co-workers reported an electrochemical aptasensor for the analysis of exosomes by hemin/G-quadruplex-assisted rolling circle amplification.¹⁸⁸ Generally, nanomaterials can act as nanocarriers, nanoelectrocatalysts and electroactive tags for signal amplification in sandwich-like electrochemical assays.

Because of their excellent biocompatibility and large surface area, AuNPs have been widely used to carry various biomolecules (such as proteins, DNA and RNA) for different biological applications. Jiang et al reported an electrochemical aptasensor for exosome detection using AuNPs and enzyme for signal amplification.¹⁸⁹ As showed in Figure 11A, aptamer-modified DNA nanotetrahedron (NTH) was employed to modify the electrode, avoiding the problem of the entanglement of aptamer and the spatial hindrance effect. Aptamer and biotin were modified on AuNPs through the interaction between

polyA₁₀ and AuNPs. After the formation of sandwich-like complexes, numerous avidin-HRP conjugates were immobilized on the biotin-labeled AuNPs to catalyze the reduction of TMB and H₂O₂.

Due to their high specific surface area, flexible porosity, and tunable framework structure, metal-organic frameworks (MOFs) have attracted wide attention in comprehensive applications, including catalysis, sensors and energy conversion and storage. The porosity endows MOFs with the ability to carry plenty of enzyme or electroactive molecules. Sun et al reported a label-free and enzyme-free electrochemical biosensor for the detection of glioblastoma-derived exosomes using Zr-based MOFs.¹⁹⁰ As displayed in Figure 11B, Zr-MOFs (UiO-66) prepared from metal ions and organic ligands through a hydrothermal method were utilized to load numerous

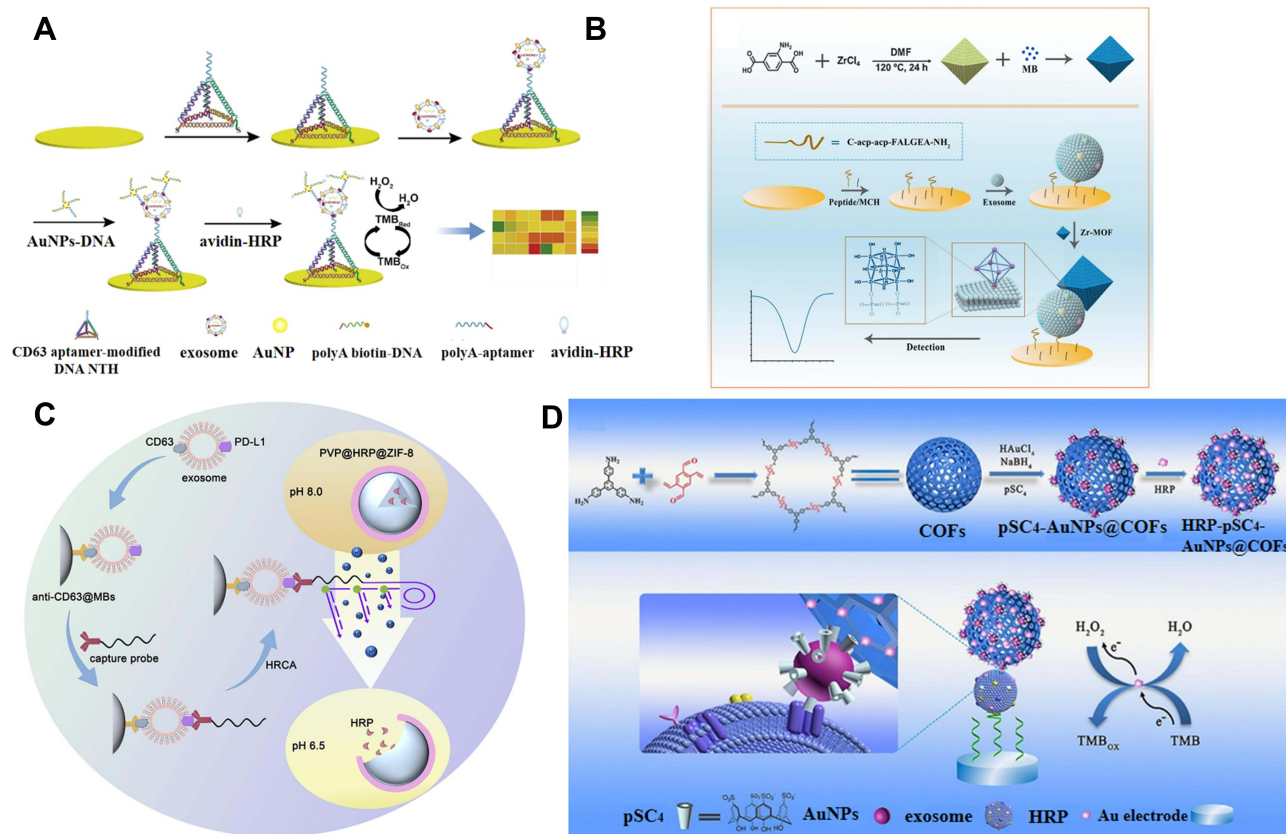


Figure 11 (A) Schematic of the electrochemical aptasensor for exosomes detection by using AuNPs and enzyme for amplification. Reprinted with permission from Jiang J, Yu Y, Zhang H, Cai C. Electrochemical aptasensor for exosomal proteins profiling based on DNA nanotetrahedron coupled with enzymatic signal amplification. *Anal Chim Acta*. 2020;1130:1–9. Copyright 2020 Elsevier B.V.¹⁸⁹ (B) Schematic of the fabrication process of MB@UiO-66-based nanoprobe and the electrochemical biosensor for the detection of GBM-derived exosomes. Reprinted with permission from Sun Z, Wang L, Wu S, et al. An electrochemical biosensor designed by using Zr-based metal-organic frameworks for the detection of glioblastoma-derived exosomes with practical application. *Anal Chem*. 2020;92:3819–3826. Copyright 2020 American Chemical Society.¹⁹⁰ (C) Schematic of identification of PD-L1⁺ exosomes based on HRCA-responsive PVP@HRP@ZIF-8. Reprinted with permission from Cao Y, Wang Y, Yu X, Jiang X, Li G, Zhao J. Identification of programmed death ligand-1 positive exosomes in breast cancer based on DNA amplification-responsive metal-organic frameworks. *Biosens Bioelectron*. 2020;166:112452–112460. Copyright 2020 Elsevier B.V.¹⁹² (D) Schematic of the fabrication process of COFs-based nanoprobe and the mechanism of the EC biosensor for exosomes detection. Reprinted with permission from Wang M, Pan Y, Wu S, et al. Detection of colorectal cancer-derived exosomes based on covalent organic frameworks. *Biosens Bioelectron*. 2020;169:112638–112645. Copyright 2020 Elsevier B.V.¹⁹³

electroactive methylene blue molecules. After the capture of exosomes by the peptide-modified electrode, methylene blue-loaded Zr-MOFs were anchored by exosomes. Zr-MOFs interacted with phosphate groups in the phospholipid bilayer of exosomes with high affinity via the formation of Zr-O-P bonds. The concentration of exosomes could be determined by measuring the electrochemical signal of methylene blue inside of MOFs. Recently, Gu et al presented a biofuel cells-based self-powered biosensor for exosome detection, in which two types of MOFs (ZIF-8 and UiO-66-NH₂) were utilized to load glucose dehydrogenase and electroactive molecules (K₃[Fe(CN)₆]), respectively.¹⁹¹ Taking the advantage of exogenous stimulus-responsive property, Cao et al reported an electrochemical biosensor for the detection of programmed death ligand-1 positive (PD-L1⁺) exosomes based on DNA amplification-responsive MOFs.¹⁹² As illustrated in Figure 11C, HRP-encapsulated ZIF-8 was prepared by biomimetic mineralization-facilitated method and then coated with PVP, which remained intact at weak alkaline pH and would be broken at acidic pH. After the capture of PD-L1⁺ exosomes by immune-MBs, the anti-PD-L1-linked DNA strands were added to label exosomes and the DNA parts initiated the hyperbranched rolling circle amplification (HRCA). The released H⁺ ions caused the

change of the environment pH to weak acidity, thus leading to the disassembly of MOFs. HRP molecules were released to increase the electrochemical response.

As an emerging kind of porous crystalline materials, covalent organic frameworks (COFs) exhibit great application potential in bioassays. Li's group reported a COFs-based aptasensor for the analysis of CRC exosomes.¹⁹³ As shown in Figure 11D, spherical COFs with high porosity were utilized to load para-sulfocalix[4]arene hydrate (pSC₄)-modified AuNPs and a large amount of HRP molecules to form HRP-pSC₄-AuNPs@COFs. pSC₄ could specifically bind with various amino acid residues on the exosome surface. AuNPs could accelerate the charge transfer of carriers. CD63 aptamer was anchored on the surface of Au electrode to capture exosomes. Then, HRP-pSC₄-AuNPs@COFs were added to recognize the captured exosomes and HRP catalyzed the oxidation of TMB by H₂O₂, generating a high electrochemical signal.

Nanozymes can catalyze the redox reaction between H₂O₂ and substrate in colorimetric assays, which can be converted into electrochemical assays with improving sensitivity. For example, Boriachek et al reported the direct isolation and subsequent detection of exosomes using gold-loaded ferric oxide nanocubes (Au-NPFe₂O₃NC).¹⁹⁴ As shown in Figure 12A, the Au-NPFe₂O₃NC was

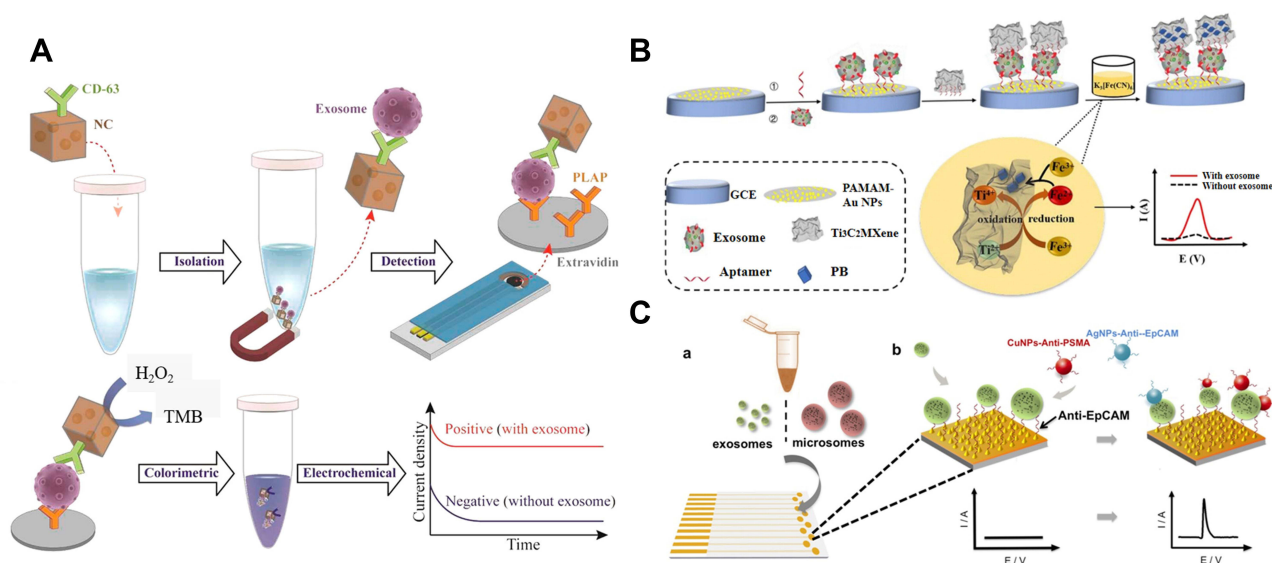


Figure 12 (A) Schematic of the assay for direct exosome isolation and detection from cell culture media based on Au-NPFe₂O₃NC. Reprinted with permission from Boriachek K, Masud MK, Palma C, et al. Avoiding pre-isolation step in exosome analysis: Direct isolation and sensitive detection of exosomes using gold-loaded nanoporous ferric oxide nanozymes. *Anal Chem*. 2019;91:3827–3834. Copyright 2019 American Chemical Society.¹⁹⁴ (B) Schematic of the electrochemical biosensor for exosomes activity detection signal amplification strategy by using in situ generation of Prussian blue. Reprinted with permission from Zhang H, Wang Z, Wang F, Zhang Y, Wang H, Liu Y. Ti3C2 MXene mediated Prussian blue in situ hybridization and electrochemical signal amplification for the detection of exosomes. *Talanta*. 2021;224:121879–121886. Copyright 2021 Elsevier B.V.¹⁹⁵ (C) Schematic representation of the two-step isolation and analysis of exosomes and microsomes: (a) capture step where vesicles are immobilized on aptamer-modified sensors, (b) electrochemical detection of the captured exosomes/microsomes with Cu and AgNPs. Reprinted with permission from Zhou YG, Mohamadi RM, Poudineh M, et al. Interrogating circulating microsomes and exosomes using metal nanoparticles. *Small*. 2016;12:727–732. Copyright 2016 Wiley-VCH.¹⁹⁷

modified with CD63 antibody for the capture of exosomes. After magnetic separation, the complex of Au-NPFe₂O₃NC and exosomes was attached on the placental alkaline phosphatase (PLAP) antibody-functionalized screen-printed electrode. The signal was measured by the Au-NPFe₂O₃NC-catalyzed reaction between TMB and H₂O₂.

Wang and co-workers developed a sensitive electrochemical biosensor for exosome detection through the in-situ generation of electroactive Prussian blue (Fe[Fe(CN)₆]) on the surface of MXenes.¹⁹⁵ As illustrated in Figure 12B, the CD63 aptamer-modified poly(amidoamine)-AuNP electrode was used to capture exosomes. Then, aptamer-conjugated MXene was used to recognize the captured exosomes. MXene on the exosome surface served as a reducing carrier to induce in-situ generation of Prussian blue, simplifying the synthesis process. Prussian Blue could produce electrochemical signal at a low potential without the interference of electroactive species. The detection limit of this method was 229 particles/μL. QDs with a large amount of metal ions can also be utilized as the signal transduction labels for the assays of exosomes.¹⁹⁶ After acid-assisted dissolution, numerous Cd²⁺ ions were released, which could be quantified by anodic stripping voltammetry (ASV). Moreover, metal NPs such as Ag and Cu can be utilized as the signal reporters because they can be directly electrochemically oxidized to produce a typical electrochemical peak. Kelley's group reported the electrochemical detection of exosomes/microsomes with anti-EpCAM aptamers-modified AgNPs and anti-PSMA aptamers-modified CuNPs (Figure 12C).¹⁹⁷ After exosomes and microsomes were captured from VCaP cells through a simple centrifugation procedure, aptamers-functionalized NPs were added to label the captured exosomes. Then, linear sweep voltammetry (LSV) was used for the direct electrochemical oxidation of AgNPs or CuNPs.

Magneto-Electrochemical Detection

The immobilization of recognition probes on the electrode may suppress the effective recognition between exosome and probe and thus decrease the sensitivity. MBs have been widely used for the capture of exosomes and can be integrated into electrochemical biosensors. MBs can not only simplify the detection procedures, but also concentrate the captured exosomes on the electrode. MBs modified with antibody (immune-MBs) have been used to isolate and enrich exosomes. MBs-based electrochemical techniques for immobilization-free detection of exosomes

have been developed.^{198,199} Lee's group designed an integrated immuno-magneto-electrochemical sensor for exosome detection (Figure 13A),²⁰⁰ in which MBs were modified with CD63 antibodies to directly capture exosomes in plasma. Next, the captured exosomes were recognized by the HRP-labeled detection antibodies. HRP could catalyze the reaction between TMB and H₂O₂, thus generating a strong electrochemical signal. To meet the need of portability and sensitivity, Ye's group reported a two-stage magnetic-based microfluidic platform for on-chip isolation and detection of exosomes.²⁰¹ As illustrated in Figure 13B, a staggered Y-shaped micropillar mixing pattern was applied to create an anisotropic flow for improving the capture efficiency. Tumor-derived exosomes captured by Tim4-coated MBs were immobilized on the ITO electrode. The ssDNA in a hairpin structure consisted of aptamer and mimicking DNAzyme sequence was employed to label exosomes. After the recognition, hairpin was opened and a G-quadruplex formed with hemin was utilized as NADH oxidase and HRP-mimicking DNAzyme simultaneously. In addition, CdSe QDs were utilized as the signal labels instead of unstable enzymes for exosome detection by an anodic stripping voltammetry.¹⁹⁶

Owing to the flexible structure, aptamer can hybridize with other DNA sequences that can initiate the DNA-based signal amplification or DNA nanomachines.^{202,203} Therefore, exosome detection can be converted into the analysis of DNA, whose amount is proportional to the number of exosomes. This strategy avoids the direct detection of exosomes on the electrode and many methods can be developed to sensitively determine DNA.²⁰⁴ For instance, Dong et al reported a highly sensitive electrochemical biosensor for exosome detection based on aptamer recognition-induced release of multi-DNA and cyclic enzymatic amplification.²⁰⁵ As shown in Figure 14A, aptamer-messenger DNA (mDNA) complexes were first modified on the MBs. LNCaP cell-derived exosomes bound to aptamer with high affinity, resulting in the release of three kinds of mDNA sequences. After the magnetic separation, the released mDNA in the supernatant initiated the Exo III-assisted cyclic enzymatic amplification reaction, leading to the sharp decrease in the amount of Ru(NH₃)₆³⁺ on the surface of Au electrode. Zhao et al reported a ratiometric electrochemical biosensor for the detection of exosomes by target-triggered 3D DNA walker and Exonuclease III-assisted cyclic enzymatic amplification.²⁰⁶ As displayed in Figure 14B, MBs were modified with high-density of DNA as 3D DNA walker

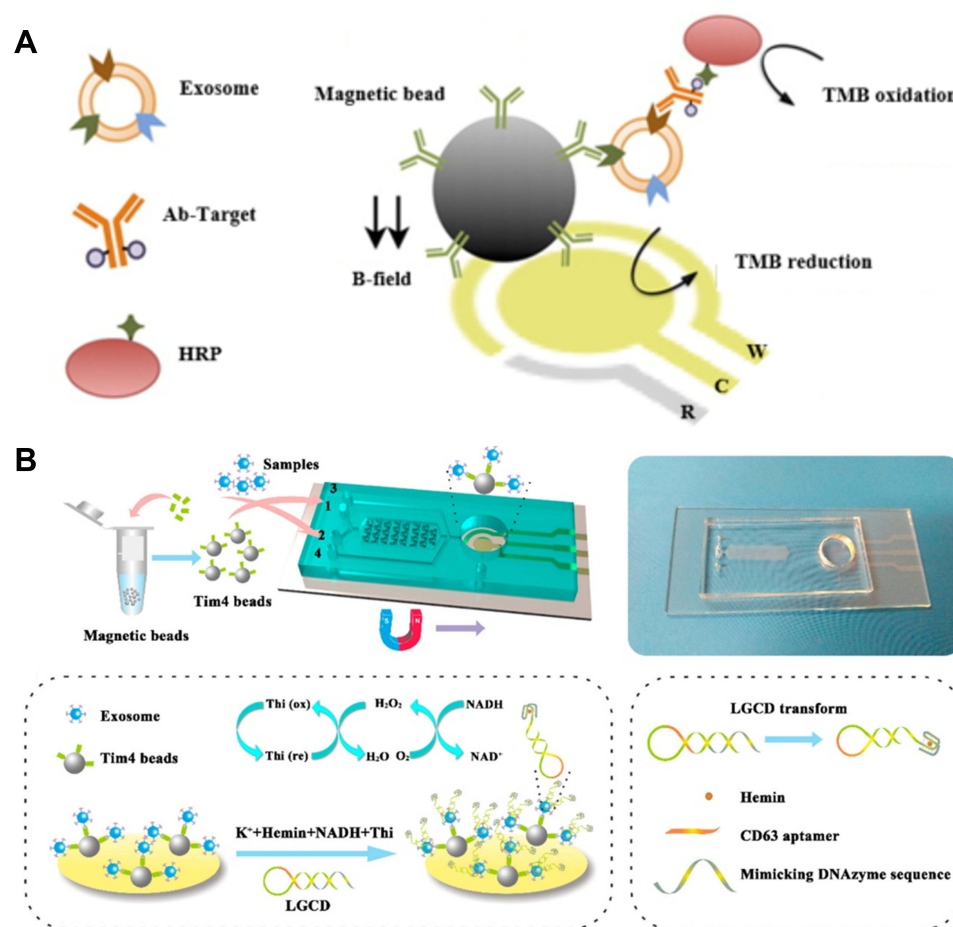


Figure 13 (A) Schematic of the integrated immuno-magneto-electrochemical sensor for exosomes detection. Reprinted with permission from Jeong S, Park J, Pathania D, et al. Integrated magneto-electrochemical sensor for exosome analysis. *ACS Nano*. 2016;10:1802–1809. Copyright 2016 American Chemical Society.²⁰⁰ **(B)** Schematic of the Exo PCD-chip and the electrochemical Sensor on the Surface of ITO Electrode. Reprinted with permission from Xu H, Liao C, Zuo P, Liu Z, Ye BC. Magnetic-based microfluidic device for on-chip isolation and detection of tumor-derived exosomes. *Anal Chem*. 2018;90:13451–13458. Copyright 2018 American Chemical Society.²⁰¹

scaffold. The DNA sequence consisted of CD63 aptamer and DNAzyme substrate. In the presence of exosomes, the recognition of CD63 aptamer on the MBs and EpCAM aptamer on the swing arm simultaneously bound to different target proteins on the same exosome, leading to the close proximity effect between DNAzyme and substrate. After the hybridization, DNA walkers were initiated and a large number of oligonucleotide fragments were released, which could be sensitively detected by the Exonuclease III-assisted cyclic enzymatic amplification.

To improve the capture efficiency, dual aptamers-modified MBs were employed to efficiently capture exosomes.²⁰⁷ As illustrated in Figure 14C, after the capture of tumor exosomes, the cholesterol-modified DNA probe was anchored on the exosome membrane through the hydrophobic interaction, triggering DNA tetrahedron-based hyperbranched HCR to generate sandwich complexes. The complexes could sequester a large amount

of $\text{Ru}(\text{NH}_3)_6^{3+}$ by electrostatic interactions, thus reducing the amount of $\text{Ru}(\text{NH}_3)_6^{3+}$ in the solution after the magnetic separation. This caused the change of current ratio of $[\text{Fe}(\text{CN})_6]^{3-}$ to $\text{Ru}(\text{NH}_3)_6^{3+}$.

Electrochemiluminescent Biosensors

As a powerful technique, ECL has been applied in various bioanalysis due to the remarkable advantages of low background signal, high sensitivity and wide detection range. To meet the need of ultrahigh sensitivity, loading of numerous luminophores into nanomaterials can boost the ECL efficiency and improve the analysis sensitivity.²⁰⁸ Feng et al designed an aptamer-binding DNA walking machine for sensitive ECL detection of tumor exosomes by employing $\text{Ru}(\text{bpy})_3^{2+}$ -loaded silica NPs as the signal reporters.²⁰⁹ To date, several nanomaterials have been utilized as the ECL emitters for diverse biosensing. For example, Sheng and co-workers developed an ECL

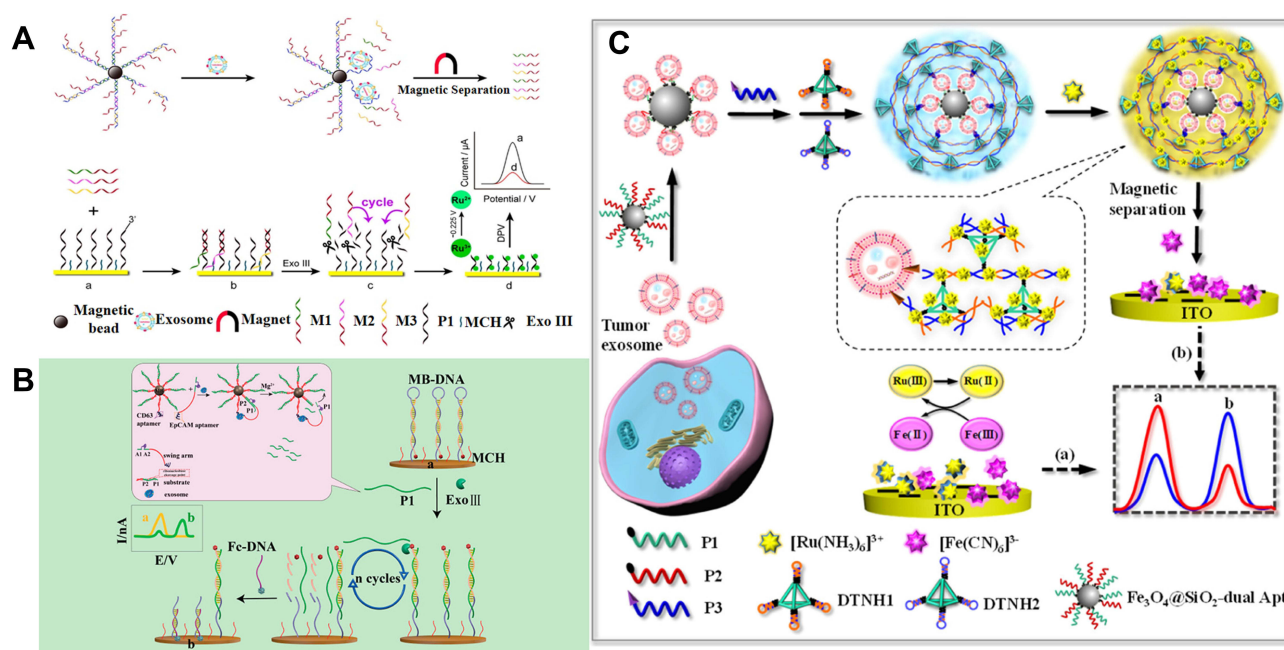


Figure 14 (A) Schematic of the highly sensitive electrochemical biosensor for exosomes detection based on aptamer recognition-induced multi-DNA release and cyclic enzymatic amplification. Reprinted with permission from Dong H, Chen H, Jiang J, Zhang H, Cai C, Shen Q. Highly sensitive electrochemical detection of tumor exosomes based on aptamer recognition-induced multi-DNA release and cyclic enzymatic amplification. *Anal Chem*. 2018;90:4507–4513. Copyright 2018 American Chemical Society.²⁰⁵ **(B)** Schematic of the ratiometric electrochemical biosensor for the detection of exosomes by target-triggered 3D DNA walker and Exo III-assisted cyclic enzymatic amplification. Reprinted with permission from Zhao L, Sun R, He P, Zhang X. Ultrasensitive detection of exosomes by target-triggered three-dimensional DNA walking machine and exonuclease III-assisted electrochemical ratiometric biosensing. *Anal Chem*. 2019;91:14773–14779. Copyright 2019 American Chemical Society.²⁰⁶ **(C)** Schematic of the ratiometric immobilization-free electrochemical sensing system for tumor exosome detection in the absence (a) and in the presence (b) of the tumor exosomes. Reprinted with permission from Yang L, Yin X, An B, Li F. Precise capture and direct quantification of tumor exosomes via a highly efficient dual-aptamer recognition-assisted ratiometric immobilization-free electrochemical strategy. *Anal Chem*. 2021;93:1709–1716. Copyright 2021 American Chemical Society.²⁰⁷

aptasensor for the analysis of exosomes by the G-quadruplex/hemin DNAzymes-induced quenching of RCL signal of Eu^{3+} -doped CdSQDs.²¹⁰ Zhang et al designed a sensitive g- C_3N_4 -coated liquid metal nanoprobe-based ECL sensing strategy for exosome detection on the multivalency interface (Figure 15A).²¹¹ In the nanoprobe, Galinstan NPs accelerated the electrode transfer and suppressed the g- C_3N_4 passivation during the electrochemical reduction processes, thus enhancing the ECL signal. Moreover, the antibody-modified PAMAM-Au NPs were used to modify the electrode for multivalent recognition of exosomes with high capture efficiency. This method achieved a detection limit of 31 particles/ μL for the determination of HeLa cell-derived exosomes. To simplify the operation procedure and reduce the contamination, Guo et al reported the QDs-based homogeneous ECL sensing of exosomes with stimuli-responsive DNA microcapsules and target recycling system.²¹² As illustrated in Figure 15B, CdS QDs-loaded CaCO_3 microcapsules were sealed by DNA-assembled stimuli-responsive shell layers. Then, the core CaCO_3 was removed by treatment with EDTA and the DNA shell-coated CdS QDs microcapsules

were formed. The presence of exosomes initiated the nicking endonuclease (Nt.BbvCI)-assisted target recycling and the crosslinked DNA shells were disintegrated. The released QDs were determined by ECL technique. The established method with dual-amplification exhibited a wide detection range of 5×10^4 to 1×10^8 particles/ μL .

Nanomaterials with excellent catalytic properties have been increasingly utilized in the development of ECL biosensors. For example, MXenes have been concerned in the areas of catalysis, biosensor and supercapacitors, owing to their excellent electron transfer ability and unique catalytic ability. Wang and co-workers reported a MXenes-catalyzed ECL biosensor for the assay of exosomes.²¹³ Fang et al proposed a self-enhanced ECL and photothermal dual-mode biosensor for exosome detection.²¹⁴ As shown in Figure 15C, MXenes were employed to carry black phosphorus (BP) quantum dots (BPQDs), $\text{Ru}(\text{dcbpy})_3^{2+}$ and CD63 antibody. In the nanocomposite, BPQDs not only catalyzed the oxidation of $\text{Ru}(\text{dcbpy})_3^{2+}$, but also acted as the coreactants. The integration of BPQDs and $\text{Ru}(\text{dcbpy})_3^{2+}$ into MXenes could shorten the distance and amplify the ECL signal.

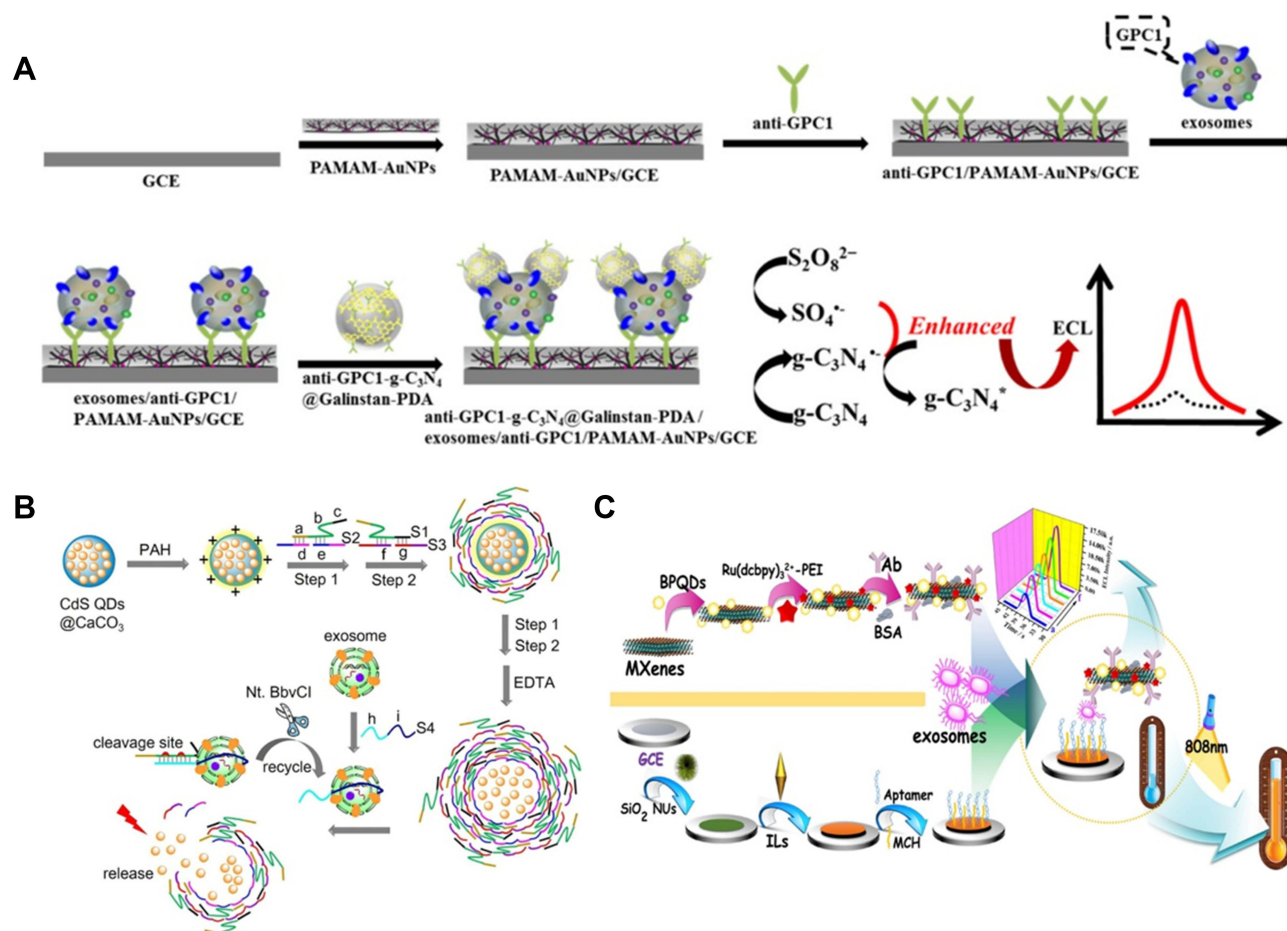


Figure 15 (A) Schematic of the ECL biosensor for exosomes based on multivalent recognition and signal amplification strategy by anti-GPC1-g-C₃N₄@Galinstan-PDA nanoprobe. Reprinted with permission from Zhang Y, Wang F, Zhang H, Wang H, Liu Y. Multivalency interface and g-C₃N₄ coated liquid metal nanoprobe signal amplification for sensitive electrogenerated chemiluminescence detection of exosomes and their surface proteins. *Anal Chem*. 2019;91:12100–12107. Copyright 2021 Elsevier B.V.²¹¹ **(B)** Schematic of the prepared process of CdS QDs-loaded DNA microcapsules integrated with target recycling amplification for homogeneous ECL detection of tumor exosomes. Reprinted with permission from Guo Y, Cao Q, Zhao C, Feng Q. Stimuli-responsive DNA microcapsules for homogeneous electrochemiluminescence sensing of tumor exosomes. *Sens Actuata B Chem*. 2021;329:129136–129142. Copyright 2019 American Chemical Society.²¹² **(C)** Schematic of the dual-mode biosensor for exosomes detection based on MXenes and black phosphorus quantum dots. Reprinted with permission from Fang D, Zhao D, Zhang S, Huang Y, Dai H, Lin Y. Black phosphorus quantum dots functionalized MXenes as the enhanced dual-mode probe for exosomes sensing. *Sens Actuata B Chem*. 2020;305:127544–127552. Copyright 2020 Elsevier B.V.²¹⁴

Moreover, both MXenes and BPQDs with good photothermal property can be used as the photothermal probes. The dual-mode biosensor exhibited a linear range of $1.1 \times 10^2 \sim 1.1 \times 10^7$ particles/ μ L. However, the stabilizers for regulating the structure and morphology and biomolecules for the specific recognition may block the active sites and hinder the electron transfer. Thus, Zhang et al reported an ECL biosensor for exosome detection based on the in-situ formation of AuNPs on the aptamer-modified MXenes (Figure 16).²¹⁵ MXenes were modified with CD63 aptamer to identify exosomes. After the capture of exosomes, aptamer-conjugated MXenes were adsorbed on the surface of exosomes. MXenes with large surface area and strong reduction ability could induce the in-situ formation of AuNPs on their surface without the addition of extra

reducing agents. AuNPs with catalytic surface greatly enhanced the ECL signal of luminol. The proposed biosensor showed a detection limit down to 30 particles/ μ L. In recent years, g-C₃N₄ was used not only as the carrier of luminol, but also as a catalyst to promote the reaction of luminol with H₂O₂, thus amplifying the ECL signal for exosome detection.²¹⁶

Photoelectrochemical Methods

A photoelectrochemical (PEC) process involves in the photocurrent as the detection signal generated by photoelectrochemically active materials under light illustration. The separation of the excitation source (light) from the detection signal (electric current) endows PEC biosensors with low background signal, high signal-to-noise ratio and

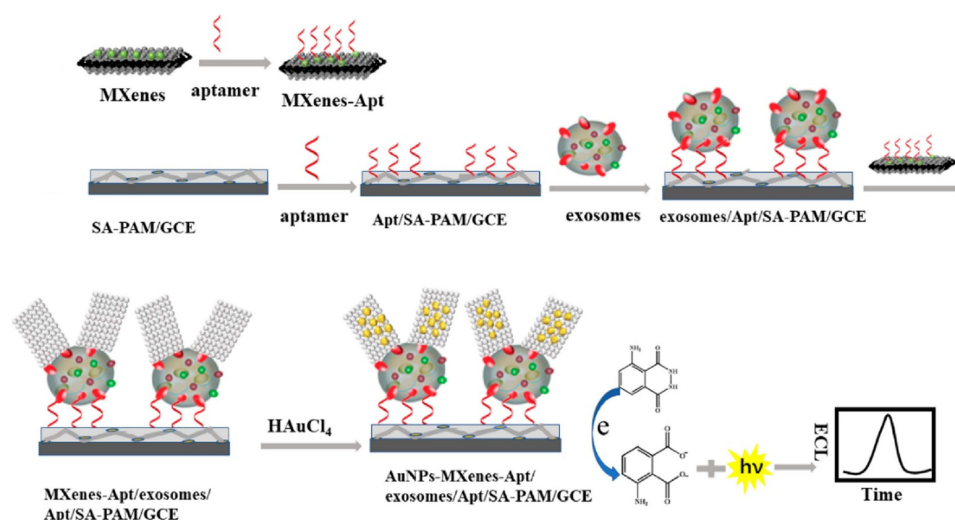


Figure 16 Schematic of the ECL biosensor for exosomes detection based on in situ formation of AuNPs decorated MXenes nanoprobe Reprinted with permission from Zhang H, Wang Z, Wang F, Zhang Y, Wang H, Liu Y. In situ formation of gold nanoparticles decorated Ti3C2 MXenes nanoprobe for highly sensitive electrogenerated chemiluminescence detection of exosomes and their surface proteins. *Anal Chem.* 2020;92:5546–5553. Copyright 2020 American Chemical Society.²¹⁵

excellent stability. Photosensitive materials play a vital role in the fabrication of PEC biosensors. Typically, Li's group designed a cathodic PEC aptasensor for the detection of exosomes using p-type NiO/BiOI/AuNP composites sensitized by CdSe QDs.²¹⁷ In this work, BiOI with a narrowbandgap (1.8 eV) was immobilized on the NiO-modified ITO to sensitize the wide band gap of NiO (3.6–4.0 eV). Then, AuNPs were deposited on the surface to conjugate EpCAM aptamers through the formation of Au-S bonds. DNA2-modified QDs were bound to the electrode surface through the hybridization, which sensitized the nanocomposite and improved the photocurrent intensity. In the presence of exosomes, aptamer bound to the EpCAM protein on the surface of exosomes, resulting in the release of QDs and the decrease of the photocurrent. Meanwhile, exosomes on the electrode surface hindered the electron transfer between electrode and electron acceptor, leading to the further attenuation of the photocurrent signal.

Other Methods

Chemiluminescence is generated from the exergonic chemical reaction, in which an intermediate molecule in singlet excited state undergoes radiative decay. Chemiluminescence biosensors can sensitively detect targets of interest in the dark without any extra input energy.²¹⁸ Zhong's group reported a chemiluminescence strategy for rapid isolation and quantification of exosomes based on CuS-enclosed microgels.²¹⁹ As displayed in

Figure 17, CuS NPs were in-situ generated in porous microgel, which further modified with streptavidin and antibody. After interaction with exosomes, microgels promoted the isolation of exosomes through membrane filtration. A large number of Cu^{2+} ions were liberated and catalyzed the reaction between H_2O_2 and luminol derivate, producing strong a chemiluminescence signal. Moreover, Wang et al reported a chemiluminescence immunoassay for exosome detection by using antibody-conjugated superparamagnetic iron oxide particles (SIOPs) and acridinium ester as the signal label.²²⁰

Mass spectrometer (MS) is an effective tool to characterize the content of biomolecules at high throughput.²²¹ However, the low sensitivity limits its utilization in detect low concentration of exosomes at the early stage of cancers. The element-labeling strategy endow MS with the advantages of high selectivity and signal amplification. In this detection principle, nanomaterials not only act as matrix materials for exosomes capture, but also can amplify MS signal due to the large amount of elements in nanomaterials.^{222–227} Recently, Zhang et al reported an ultrasensitive inductively coupled plasma-mass spectrometry (ICP-MS) method for the detection of exosomes by using UCNPs as element labels.²²⁸ As shown in Figure 18, three different elements (Y, Eu, and Tb) doped UCNPs modified with three different aptamers were linked to AuNPs, forming three satellite-like nanoassemblies. Exosomes with surface proteins could trigger the release of the corresponding

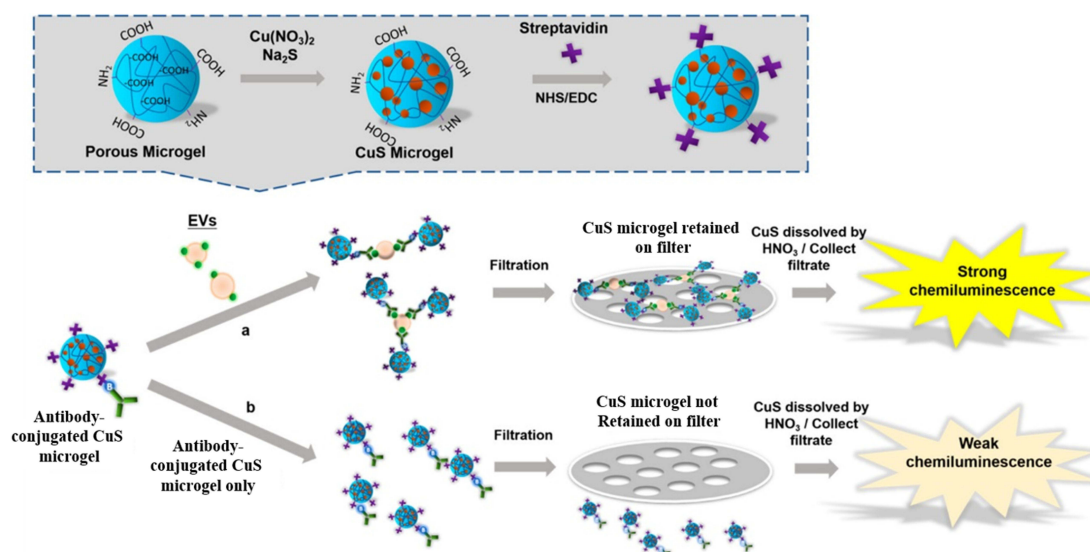


Figure 17 Schematic of CuS-microgel synthesis and the CuS-microgel-based assay for exosome quantification. Reprinted with permission from Jiang Q, Liu Y, Wang L, Adkins GB, Zhong W. Rapid enrichment and detection of extracellular vesicles enabled by cus-enclosed microgels. *Anal Chem.* 2019;91:15951–15958. Copyright 2019 American Chemical Society.²¹⁹

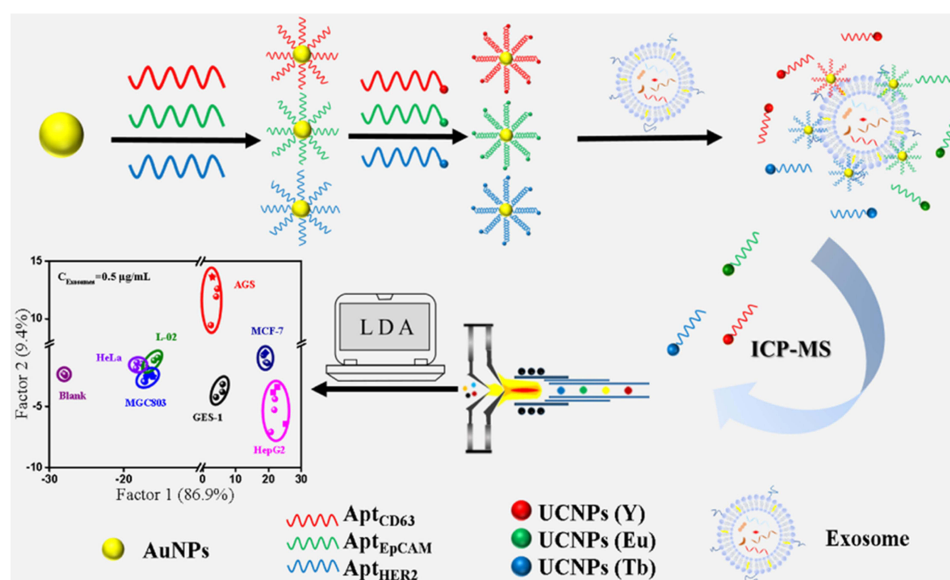


Figure 18 Schematic of ultrasensitive inductively coupled plasma-mass spectrometry method for the detection of exosomes by using UCNPs as element labels. Reprinted with permission from Zhang XW, Liu MX, He MQ, Chen S, Yu YL, Wang JH. Integral multielement signals by DNA-programmed UCNPs-AuNP nanosatellite assemblies for ultrasensitive ICP-MS detection of exosomal proteins and cancer identification. *Anal Chem.* 2021;93:6437–6445. Copyright 2021 American Chemical Society.²²⁸

aptamers conjugated with UCNPs from AuNPs. Then, the released UCNPs in solution were detected by ICP-MS. Finally, this sensitive and high-throughput method could distinguish exosomes from seven different cell lines.

Conclusions

In this review, we have systematically reviewed various nanomaterials-based techniques for exosome detection.

The unique characteristics of nanomaterials make them fascinating materials for signal transduction and biosensor development. Moreover, the sensitivity and selectivity of biosensors for exosome detection have greatly improved by integration with various elaborate DNA or enzyme-based signal amplification strategies. In spite of significant progress in exosome detection, there are still some challenges to be addressed. For example, stability of nanomaterials and

selectivity for complex samples should be improved by appropriate modification with biocompatibility polymers or others. Biorecognition elements used in bioassays may suffer from the digestion of enzymes in real samples. For transforming research in laboratory into clinical practice, it is the key obstacle to develop standardized technical specifications, including collection of biological samples, isolation of exosomes from liposy and detection operation. It is beneficial to enhance the comparability of results and establish a reliable and comprehensive dataset for future study on exosomes. The cost-effective and high-throughput isolation and detection of exosomes is helpful to simultaneously identify a large amount of clinical samples. We believe that nanomaterials-based detection of exosomes will make greater progress with the collective and unremitting efforts of different fields such as chemistry, materials science and clinical diagnosis.

Funding

This research was funded by the Program for Innovative Research Team of Science and Technology in the University of Henan Province (21IRTSTHN005), the National Natural Science Foundation of China (21804085), and the Research Funds for the Henan Key Laboratory of Biomolecular Recognition and Sensing (HKLBRK1902).

Disclosure

The authors declare no conflict of interest.

References

- Harding C, Stahl P. Transferrin recycling in reticulocytes: pH and iron are important determinants of ligand binding and processing. *Biochem Biophys Res Commun.* 1983;113:650–658. doi:10.1016/0006-291X(83)91776-X
- Wang H, Chen K, Yang Z, et al. Diagnosis of invasive nonfunctional pituitary adenomas by serum extracellular vesicles. *Anal Chem.* 2019;91:9580–9589. doi:10.1021/acs.analchem.9b00914
- Thery C, Witwer KW, Aikawa E, et al. Minimal information for studies of extracellular vesicles 2018 (misev2018): a position statement of the international society for extracellular vesicles and update of the misev2014 guidelines. *J Extracell Vesicles.* 2018;7:1535750.
- Yan H, Li Y, Cheng S, Zeng Y. Advances in analytical technologies for extracellular vesicles. *Anal Chem.* 2021;93:4739–4774. doi:10.1021/acs.analchem.1c00693
- Hyun KA, Kim J, Gwak H, Jung HI. Isolation and enrichment of circulating biomarkers for cancer screening, detection, and diagnostics. *Analyst.* 2016;141:382–392. doi:10.1039/C5AN01762A
- Jeppesen DK, Fenix AM, Franklin JL, et al. Reassessment of exosome composition. *Cell.* 2019;177:428–445. doi:10.1016/j.cell.2019.02.029
- Gurunathan S, Kang MH, Kim JH. A comprehensive review on factors influences biogenesis, functions, therapeutic and clinical implications of exosomes. *Int J Nanomed.* 2021;16:1281–1312. doi:10.2147/IJN.S291956
- Lee Y, El Andaloussi S, Wood MJ, et al. Exosomes and microvesicles: extracellular vesicles for genetic information transfer and gene therapy. *Hum Mol Genet.* 2012;21:R125–R134. doi:10.1093/hmg/dds317
- Kalluri R, LeBleu VS. The biology, function, and biomedical applications of exosomes. *Science.* 2020;367:6697–6712. doi:10.1126/science.aau6977
- Al-Nedawi K, Meehan B, Micallef J, et al. Intercellular transfer of the oncogenic receptor egfrviii by microvesicles derived from tumour cells. *Nat Cell Biol.* 2008;10:619–624. doi:10.1038/ncb1725
- Peinado H, Aleckovic M, Lavotshkin S, et al. Melanoma exosomes educate bone marrow progenitor cells toward a pro-metastatic phenotype through MET. *Nat Med.* 2012;18:883–891. doi:10.1038/nm.2753
- Chen C, Skog J, Hsu CH, et al. Microfluidic isolation and transcriptome analysis of serum microvesicles. *Lab Chip.* 2010;10:505–511. doi:10.1039/B916199F
- Ale Ebrahim S, Ashtari A, Zamani Pedram M, Ale Ebrahim N, Sanati-Nezhad A. Publication trends in exosomes nanoparticles for cancer detection. *Int J Nanomed.* 2020;15:4453–4470. doi:10.2147/IJN.S247210
- LeBleu VS, Kalluri R. Exosomes as a multicomponent biomarker platform in cancer. *Trends Cancer.* 2020;6:767–774. doi:10.1016/j.trecan.2020.03.007
- Hoshino A, Kim HS, Bojmar L, et al. Extracellular vesicle and particle biomarkers define multiple human cancers. *Cell.* 2020;182:1044–1061. doi:10.1016/j.cell.2020.07.009
- Bhat EA, Sajjad N, Thokar FM. Current advancement of exosomes as biomarkers for cancer diagnosis and forecasting. *Cancer Treat Res Commun.* 2021;28:100417. doi:10.1016/j.ctarc.2021.100417
- Kok VC, Yu CC. Cancer-derived exosomes: their role in cancer biology and biomarker development. *Int J Nanomed.* 2020;15:8019–8036. doi:10.2147/IJN.S272378
- Woo HK, Sunkara V, Park J, et al. Exodisc for rapid, size-selective, and efficient isolation and analysis of nanoscale extracellular vesicles from biological samples. *ACS Nano.* 2017;11:1360–1370. doi:10.1021/acsnano.6b06131
- Clayton A, Court J, Navabi H, et al. Analysis of antigen presenting cell derived exosomes, based on immuno-magnetic isolation and flow cytometry. *J Immunol Methods.* 2001;247:163–174. doi:10.1016/S0022-1759(00)00321-5
- Busatto S, Giacomini A, Montis C, Ronca R, Bergese P. Uptake profiles of human serum exosomes by murine and human tumor cells through combined use of colloidal nanoplasmonics and flow cytofluorimetric analysis. *Anal Chem.* 2018;90:7855–7861. doi:10.1021/acs.analchem.7b04374
- Zhou H, Yuen PS, Pisitkun T, et al. Collection, storage, preservation, and normalization of human urinary exosomes for biomarker discovery. *Kidney Int.* 2006;69:1471–1476. doi:10.1038/sj.ki.5000273
- van der Pol E, Hoekstra AG, Sturk A, Otto C, van Leeuwen TG, Nieuwland R. Optical and non-optical methods for detection and characterization of microparticles and exosomes. *J Thromb Haemost.* 2010;8:2596–2607. doi:10.1111/j.1538-7836.2010.04074.x
- Sun Y, Haglund TA, Rogers AJ, Ghanim AF, Sethu P. Review: microfluidics technologies for blood-based cancer liquid biopsies. *Anal Chim Acta.* 2018;1012:10–29. doi:10.1016/j.aca.2017.12.050
- Salomon C, Kobayashi M, Ashman K, Sobrevia L, Mitchell MD, Rice GE. Hypoxia-induced changes in the bioactivity of cytotrophoblast-derived exosomes. *PLoS One.* 2013;8:79636–79650. doi:10.1371/journal.pone.0079636
- Kim D, Woo HK, Lee C, et al. EV-Ident: identifying tumor-specific extracellular vesicles by size fractionation and single-vesicle analysis. *Anal Chem.* 2020;92:6010–6018. doi:10.1021/acs.analchem.0c00285

26. Zhang J, Shi J, Liu W, et al. A simple, specific and “on-off” type MUC1 fluorescence aptasensor based on exosomes for detection of breast cancer. *Sens Actuat B Chem.* 2018;276:552–559. doi:10.1016/j.snb.2018.08.056
27. Zhao W, Cui CH, Bose S, et al. Bioinspired multivalent DNA network for capture and release of cells. *Proc Natl Acad Sci U S A.* 2012;109:19626–19631. doi:10.1073/pnas.1211234109
28. Xiao D, Ohlendorf J, Chen Y, et al. Identifying mRNA, microRNA and protein profiles of melanoma exosomes. *PLoS One.* 2012;7:46874–46889. doi:10.1371/journal.pone.0046874
29. Akbarinejad A, Hissey CL, Brewster D, et al. Novel electrochemically switchable, flexible, microporous cloth that selectively captures, releases, and concentrates intact extracellular vesicles. *ACS Appl Mater Interfaces.* 2020;12:39005–39013. doi:10.1021/acsami.0c11908
30. Liu C, Qie Y, Qin W, et al. Emerging immunoassay technologies for the rapid detection of exosomes. *Sens Actuat B Chem.* 2021;345:130336–130351. doi:10.1016/j.snb.2021.130336
31. Ziaei P, Berkman CE, Norton MG. Review: isolation and detection of tumor-derived extracellular vesicles. *ACS Appl Nano Mater.* 2018;1:2004–2020. doi:10.1021/acsanm.8b00267
32. Dong J, Zhang RY, Sun N, et al. Bio-inspired nanovilli chips for enhanced capture of tumor-derived extracellular vesicles: toward non-invasive detection of gene alterations in non-small cell lung cancer. *ACS Appl Mater Interfaces.* 2019;11:13973–13983. doi:10.1021/acsami.9b01406
33. Yang Y, Kannisto E, Yu G, Reid ME, Patnaik SK, Wu Y. An immuno-biochip selectively captures tumor-derived exosomes and detects exosomal RNAs for cancer diagnosis. *ACS Appl Mater Interfaces.* 2018;10:43375–43386. doi:10.1021/acsami.8b13971
34. Ibsen SD, Wright J, Lewis JM, et al. Rapid isolation and detection of exosomes and associated biomarkers from plasma. *ACS Nano.* 2017;11:6641–6651. doi:10.1021/acsnano.7b00549
35. Zhao Z, Yang Y, Zeng Y, He M. A microfluidic exosearch chip for multiplexed exosome detection towards blood-based ovarian cancer diagnosis. *Lab Chip.* 2016;16:489–496. doi:10.1039/C5LC01117E
36. Lin S, Yu Z, Chen D, et al. Progress in microfluidics-based exosome separation and detection technologies for diagnostic applications. *Small.* 2020;16:1903916. doi:10.1002/smll.201903916
37. Kang YT, Hadlock T, Jolly S, Nagrath S. Extracellular vesicles on demand (EVOD) chip for screening and quantification of cancer-associated extracellular vesicles. *Biosens Bioelectron.* 2020;168:112535. doi:10.1016/j.bios.2020.112535
38. Kang YT, Purcell E, Palacios-Rolston C, et al. Isolation and profiling of circulating tumor-associated exosomes using extracellular vesicular lipid-protein binding affinity based microfluidic device. *Small.* 2019;15:e1903600. doi:10.1002/smll.201903600
39. Ding L, Yang X, Gao Z, et al. A holistic review of the state-of-the-art microfluidics for exosome separation: an overview of the current status, existing obstacles, and future outlook. *Small.* 2021;17:e2007174. doi:10.1002/smll.202007174
40. Rana A, Zhang Y, Esfandiari L. Advancements in microfluidic technologies for isolation and early detection of circulating cancer-related biomarkers. *Analyst.* 2018;143:2971–2991. doi:10.1039/C7AN01965C
41. Zhang P, Zhou X, He M, et al. Ultrasensitive detection of circulating exosomes with a 3D-nanopatterned microfluidic chip. *Nat Biomed Eng.* 2019;3:438–451. doi:10.1038/s41551-019-0356-9
42. Su W, Li H, Chen W, Qin J. Microfluidic strategies for label-free exosomes isolation and analysis. *TrAC Trends Anal Chem.* 2019;118:686–698. doi:10.1016/j.trac.2019.06.037
43. Wang Y, Li Q, Shi H, et al. Microfluidic Raman biochip detection of exosomes: a promising tool for prostate cancer diagnosis. *Lab Chip.* 2020;20:4632–4637. doi:10.1039/D0LC00677G
44. Yang Q, Cheng L, Hu L, et al. An integrative microfluidic device for isolation and ultrasensitive detection of lung cancer-specific exosomes from patient urine. *Biosens Bioelectron.* 2020;163:112290. doi:10.1016/j.bios.2020.112290
45. Zhu C, Li L, Wang Z, Irfan M, Qu F. Recent advances of aptasensors for exosomes detection. *Biosens Bioelectron.* 2020;160:112213. doi:10.1016/j.bios.2020.112213
46. Zhang K, Yue Y, Wu S, Liu W, Shi J, Zhang Z. Rapid capture and nondestructive release of extracellular vesicles using aptamer-based magnetic isolation. *ACS Sens.* 2019;4:1245–1251. doi:10.1021/acssensors.9b00060
47. Suwathanarak T, Thiodorus IA, Tanaka M, et al. Microfluidic-based capture and release of cancer-derived exosomes via peptide-nanowire hybrid interface. *Lab Chip.* 2021;21:597–607. doi:10.1039/D0LC00899K
48. Feng Y, Guo Y, Li Y, et al. Lectin-mediated in situ rolling circle amplification on exosomes for probing cancer-related glycan pattern. *Anal Chim Acta.* 2018;1039:108–115. doi:10.1016/j.aca.2018.07.040
49. Choi Y, Park U, Koo HJ, et al. Exosome-mediated diagnosis of pancreatic cancer using lectin-conjugated nanoparticles bound to selective glycans. *Biosens Bioelectron.* 2021;177:112980–112990. doi:10.1016/j.bios.2021.112980
50. Zhang P, Dong B, Zeng E, et al. In vivo tracking of multiple tumor exosomes labeled by phospholipid-based bioorthogonal conjugation. *Anal Chem.* 2018;90:11273–11279. doi:10.1021/acs.analchem.8b01506
51. Zhang W, Yu ZL, Wu M, et al. Magnetic and folate functionalization enables rapid isolation and enhanced tumor-targeting of cell-derived microvesicles. *ACS Nano.* 2017;11:277–290. doi:10.1021/acsnano.6b05630
52. Shao H, Im H, Castro CM, Breakefield X, Weissleder R, Lee H. New technologies for analysis of extracellular vesicles. *Chem Rev.* 2018;118:1917–1950. doi:10.1021/acs.chemrev.7b00534
53. Cheng N, Du D, Wang X, et al. Recent advances in biosensors for detecting cancer-derived exosomes. *Trends Biotechnol.* 2019;37:1236–1254. doi:10.1016/j.tibtech.2019.04.008
54. Kholafazad Kordasht H, Hasanzadeh M. Biomedical analysis of exosomes using biosensing methods: recent progress. *Anal Methods.* 2020;12:2795–2811. doi:10.1039/D0AY00722F
55. Xu H, Ye B-C. Advances in biosensing technologies for analysis of cancer-derived exosomes. *TrAC Trend Anal Chem.* 2020;123:115773–115784. doi:10.1016/j.trac.2019.115773
56. Shao B, Xiao Z. Recent achievements in exosomal biomarkers detection by nanomaterials-based optical biosensors - a review. *Anal Chim Acta.* 2020;1114:74–84. doi:10.1016/j.aca.2020.02.041
57. Yu X, Sha L, Dong L, Cao Y, Zhao J. Recent advances in bio-sensing methods for the detection of tumor exosomes. *Crit Rev Anal Chem.* 2020;1–19. doi:10.1080/10408347.2020.1802220
58. Zhang L, Gu C, Wen J, Liu G, Liu H, Li L. Recent advances in nanomaterial-based biosensors for the detection of exosomes. *Anal Bioanal Chem.* 2021;413:83–102. doi:10.1007/s00216-020-03000-0
59. Xiong H, Huang Z, Yang Z, et al. Recent progress in detection and profiling of cancer cell-derived exosomes. *Small.* 2021;17(35):2007971. doi:10.1002/smll.202007971
60. Liu C, Xu X, Li B, et al. Single-exosome-counting immunoassays for cancer diagnostics. *Nano Lett.* 2018;18:4226–4232. doi:10.1021/acs.nanolett.8b01184
61. Kashefi-Kheyabadi L, Kim J, Chakravarty S, et al. Detachable microfluidic device implemented with electrochemical aptasensor (DeMEA) for sequential analysis of cancerous exosomes. *Biosens Bioelectron.* 2020;169:112622–112631. doi:10.1016/j.bios.2020.112622

62. Tayebi M, Zhou Y, Tripathi P, Chandramohanadas R, Ai Y. Exosome purification and analysis using a facile microfluidic hydrodynamic trapping device. *Anal Chem*. 2020;92:10733–10742. doi:10.1021/acs.analchem.0c02006
63. Zhou S, Hu T, Zhang F, et al. Integrated microfluidic device for accurate extracellular vesicle quantification and protein markers analysis directly from human whole blood. *Anal Chem*. 2020;92:1574–1581.
64. Mohammadi M, Zargartalebi H, Salahandish R, Aburashed R, Wey Yong K, Sanati-Nezhad A. Emerging technologies and commercial products in exosome-based cancer diagnosis and prognosis. *Biosens Bioelectron*. 2021;183:113176–113203.
65. Liu C, Zhao J, Tian F, Chang J, Zhang W, Sun J. Lambda-DNA- and aptamer-mediated sorting and analysis of extracellular vesicles. *J Am Chem Soc*. 2019;141:3817–3821. doi:10.1021/jacs.9b00007
66. Li Q, Wang Y, Ling L, et al. Rapid and specific detection nanoplat-form of serum exosomes for prostate cancer diagnosis. *Microchim Acta*. 2021;188:283–293. doi:10.1007/s00604-021-04934-7
67. Zhand S, Xiao K, Razavi Bazaz S, et al. Improving capture efficiency of human cancer cell derived exosomes with nanostructured metal organic framework functionalized beads. *Appl Mater Today*. 2021;23:100994–101007. doi:10.1016/j.apmt.2021.100994
68. Thorsteinsson K, Olsen E, Schmidt E, Pace H, Bally M. FRET-based assay for the quantification of extracellular vesicles and other vesicles of complex composition. *Anal Chem*. 2020;92:15336–15343. doi:10.1021/acs.analchem.0c02271
69. Lyu Y, Cui D, Huang J, Fan W, Miao Y, Pu K. Near-infrared afterglow semiconducting nano-polycomplexes for the multiplex differentiation of cancer exosomes. *Angew Chem Int Ed*. 2019;58:4983–4987. doi:10.1002/anie.201900092
70. Li N, Huang Z, Zhang X, Song X, Xiao Y. Reflecting size differences of exosomes by using the combination of membrane-targeting viscosity probe and fluorescence lifetime imaging microscopy. *Anal Chem*. 2019;91:15308–15316. doi:10.1021/acs.analchem.9b04587
71. Wang F, Zhang Y, Chen D, Zhang Z, Li Z. Single microbead-based fluorescent aptasensor (SMFA) for direct isolation and in situ quantification of exosomes from plasma. *Analyst*. 2021;146:3346–3351. doi:10.1039/D1AN00463H
72. Xu R, Fitts A, Li X, et al. Quantification of small extracellular vesicles by size exclusion chromatography with fluorescence detection. *Anal Chem*. 2016;88:10390–10394. doi:10.1021/acs.analchem.6b03348
73. Lazaro-Ibanez E, Faruqu FN, Saleh AF, et al. Selection of fluorescent, bioluminescent, and radioactive tracers to accurately reflect extracellular vesicle biodistribution in vivo. *ACS Nano*. 2021;15:3212–3227. doi:10.1021/acsnano.0c09873
74. Fujii T, Kaneta T. Direct counting of exosomes in a cell culture medium using neither isolation nor preconcentration. *Anal Chim Acta*. 2020;1119:35–40. doi:10.1016/j.aca.2020.04.052
75. Wang L, Yang Y, Liu Y, Ning L, Xiang Y, Li G. Bridging exosome and liposome through zirconium-phosphate coordination chemistry: a new method for exosome detection. *Chem Commun*. 2019;55:2708–2711. doi:10.1039/C9CC00220K
76. Zhang P, He M, Zeng Y. Ultrasensitive microfluidic analysis of circulating exosomes using a nanostructured graphene oxide/polydopamine coating. *Lab Chip*. 2016;16:3033–3042. doi:10.1039/C6LC00279J
77. Wan S, Zhang L, Wang S, et al. Molecular recognition-based DNA nanoassemblies on the surfaces of nanosized exosomes. *J Am Chem Soc*. 2017;139:5289–5292. doi:10.1021/jacs.7b00319
78. He D, Ho SL, Chan HN, et al. Molecular-recognition-based DNA nanodevices for enhancing the direct visualization and quantification of single vesicles of tumor exosomes in plasma microsamples. *Anal Chem*. 2019;91:2768–2775. doi:10.1021/acs.analchem.8b04509
79. Tian Q, He C, Liu G, et al. Nanoparticle counting by microscopic digital detection: selective quantitative analysis of exosomes via surface-anchored nucleic acid amplification. *Anal Chem*. 2018;90:6556–6562.
80. Zhao X, Zeng L, Mei Q, Luo Y. Allosteric probe-initiated wash-free method for sensitive extracellular vesicle detection through dual cycle-assisted CRISPR-Cas12a. *ACS Sens*. 2020;5:2239–2246. doi:10.1021/acssensors.0c00944
81. Chen J, Meng HM, An Y, et al. Structure-switching aptamer triggering hybridization displacement reaction for label-free detection of exosomes. *Talanta*. 2020;209:120510–120517. doi:10.1016/j.talanta.2019.120510
82. Wang L, Pan Y, Liu Y, et al. Fabrication of an aptamer-coated liposome complex for the detection and profiling of exosomes based on terminal deoxynucleotidyl transferase-mediated signal amplification. *ACS Appl Mater Interfaces*. 2020;12:322–329. doi:10.1021/acsami.9b18869
83. Shi L, Ba L, Xiong Y, Peng G. A hybridization chain reaction based assay for fluorometric determination of exosomes using magnetic nanoparticles and both aptamers and antibody as recognition elements. *Microchim Acta*. 2019;186:796–802. doi:10.1007/s00604-019-3823-9
84. Wang X, Shang H, Ma C, Chen L. A fluorescence assay for exosome detection based on bivalent cholesterol anchor triggered target conversion and enzyme-free signal amplification. *Anal Chem*. 2021;93:8493–8500. doi:10.1021/acs.analchem.1c00796
85. Yu X, He L, Pentok M, et al. An aptamer-based new method for competitive fluorescence detection of exosomes. *Nanoscale*. 2019;11:15589–15595. doi:10.1039/C9NR04050A
86. Zhang H, Zhou Y, Luo D, et al. Immunoassay-aptasensor for the determination of tumor-derived exosomes based on the combination of magnetic nanoparticles and hybridization chain reaction. *RSC Adv*. 2021;11:4983–4990. doi:10.1039/D0RA10159A
87. Wang H, Wan K, Zhou Y, et al. A three-dimensional multipedal DNA walker for the ultrasensitive detection of tumor exosomes. *Chem Commun*. 2020;56:12949–12952. doi:10.1039/D0CC04360E
88. Huang L, Wang DB, Singh N, Yang F, Gu N, Zhang XE. A dual-signal amplification platform for sensitive fluorescence biosensing of leukemia-derived exosomes. *Nanoscale*. 2018;10:20289–20295. doi:10.1039/C8NR07720G
89. Huang Z, Lin Q, Yang B, et al. Cascade signal amplification for sensitive detection of exosomes by integrating tyramide and surface-initiated enzymatic polymerization. *Chem Commun*. 2020;56:12793–12796. doi:10.1039/D0CC04881J
90. Gao ML, He F, Yin BC, Ye BC. A dual signal amplification method for exosome detection based on DNA dendrimer self-assembly. *Analyst*. 2019;144:1995–2002. doi:10.1039/C8AN02383B
91. Pan Y, Wang L, Deng Y, et al. A simple and sensitive method for exosome detection based on steric hindrance-controlled signal amplification. *Chem Commun*. 2020;56:13768–13771. doi:10.1039/D0CC06113A
92. Li P, Yu X, Han W, et al. Ultrasensitive and reversible nanoplat-form of urinary exosomes for prostate cancer diagnosis. *ACS Sens*. 2019;4:1433–1441. doi:10.1021/acssensors.9b00621
93. Dobhal G, Ayupova D, Laufersky G, Ayed Z, Nann T, Goreham RV. Cadmium-free quantum dots as fluorescent labels for exosomes. *Sensors*. 2018;18:3308–3320. doi:10.3390/s18103308
94. Zhu N, Li G, Zhou J, et al. A light-up fluorescence resonance energy transfer magnetic aptamer-sensor for ultra-sensitive lung cancer exosome detection. *J Mater Chem B*. 2021;9:2483–2493. doi:10.1039/D1TB00046B
95. Wu M, Chen Z, Xie Q, et al. One-step quantification of salivary exosomes based on combined aptamer recognition and quantum dot signal amplification. *Biosens Bioelectron*. 2021;171:112733–112742. doi:10.1016/j.bios.2020.112733

96. Zhang J, Zhu Y, Shi J, Zhang K, Zhang Z, Zhang H. Sensitive signal amplifying a diagnostic biochip based on a biomimetic periodic nanostructure for detecting cancer exosomes. *ACS Appl Mater Interfaces*. 2020;12:33473–33482. doi:10.1021/acsami.0c06785
97. Dong D, Zhu L, Hu J, Pang DW, Zhang ZL. Simple and rapid extracellular vesicles quantification via membrane biotinylation strategy coupled with fluorescent nanospheres-based lateral flow assay. *Talanta*. 2019;200:408–414. doi:10.1016/j.talanta.2019.03.069
98. He F, Wang J, Yin BC, Ye BC. Quantification of exosome based on a copper-mediated signal amplification strategy. *Anal Chem*. 2018;90:8072–8079. doi:10.1021/acs.analchem.8b01187
99. Yu Y, Zhang WS, Guo Y, et al. Engineering of exosome-triggered enzyme-powered DNA motors for highly sensitive fluorescence detection of tumor-derived exosomes. *Biosens Bioelectron*. 2020;167:112482–112490. doi:10.1016/j.bios.2020.112482
100. Chen X, Lan J, Liu Y, et al. A paper-supported aptasensor based on upconversion luminescence resonance energy transfer for the accessible determination of exosomes. *Biosens Bioelectron*. 2018;102:582–588. doi:10.1016/j.bios.2017.12.012
101. Jin D, Yang F, Zhang Y, et al. Exoapp: exosome-oriented, aptamer nanoprobe-enabled surface proteins profiling and detection. *Anal Chem*. 2018;90:14402–14411. doi:10.1021/acs.analchem.8b03959
102. Wang H, Chen H, Huang Z, Li T, Deng A, Kong J. DNase I enzyme-aided fluorescence signal amplification based on graphene oxide-DNA aptamer interactions for colorectal cancer exosome detection. *Talanta*. 2018;184:219–226. doi:10.1016/j.talanta.2018.02.083
103. Li B, Pan W, Liu C, et al. Homogenous magneto-fluorescent nanosensor for tumor-derived exosome isolation and analysis. *ACS Sens*. 2020;5:2052–2060. doi:10.1021/acssensors.0c00513
104. Tayebi M, Tavakkoli Yarak M, Yang HY, Ai Y. A mos2–mwcnt based fluorometric nanosensor for exosome detection and quantification. *Nanoscale Adv*. 2019;1:2866–2872. doi:10.1039/C9NA00248K
105. Zhang Q, Wang F, Zhang H, Zhang Y, Liu M, Liu Y. Universal Ti3C2 MXenes based self-standard ratiometric fluorescence resonance energy transfer platform for highly sensitive detection of exosomes. *Anal Chem*. 2018;90:12737–12744. doi:10.1021/acs.analchem.8b03083
106. Lee J, Kim H, Heo Y, et al. Enhanced paper-based ELISA for simultaneous EVs/exosome isolation and detection using streptavidin agarose-based immobilization. *Analyst*. 2019;145:157–164. doi:10.1039/C9AN01140D
107. Xia Y, Chen T, Chen G, et al. A nature-inspired colorimetric and fluorescent dual-modal biosensor for exosomes detection. *Talanta*. 2020;214:120851–120861. doi:10.1016/j.talanta.2020.120851
108. Hartman ZC, Wei J, Glass OK, et al. Increasing vaccine potency through exosome antigen targeting. *Vaccine*. 2011;29:9361–9367. doi:10.1016/j.vaccine.2011.09.133
109. Khodashenas S, Khalili S, Forouzandeh Moghadam M. A cell ELISA based method for exosome detection in diagnostic and therapeutic applications. *Biotechnol Lett*. 2019;41:523–531. doi:10.1007/s10529-019-02667-5
110. Logozzi M, De Milito A, Lugini L, et al. High levels of exosomes expressing CD63 and caveolin-1 in plasma of melanoma patients. *PLoS One*. 2009;4:5219–5229. doi:10.1371/journal.pone.0005219
111. Zhou Y, Xu H, Wang H, Ye BC. Detection of breast cancer-derived exosomes using the horseradish peroxidase-mimicking dnazyme as an aptasensor. *Analyst*. 2019;145:107–114. doi:10.1039/C9AN01653H
112. Xu H, Zheng L, Zhou Y, Ye B-C. An artificial enzyme cascade amplification strategy for highly sensitive and specific detection of breast cancer-derived exosomes. *Analyst*. 2021;146(18):5542–5549. doi:10.1039/d1an01071a
113. Chen Z, Cheng SB, Cao P, et al. Detection of exosomes by ZnO nanowires coated three-dimensional scaffold chip device. *Biosens Bioelectron*. 2018;122:211–216. doi:10.1016/j.bios.2018.09.033
114. Huang Z, Lin Q, Ye X, et al. Terminal deoxynucleotidyl transferase based signal amplification for enzyme-linked aptamer-sorbent assay of colorectal cancer exosomes. *Talanta*. 2020;218:121089–121097. doi:10.1016/j.talanta.2020.121089
115. Moura SL, Martin CG, Marti M, Pividori MI. Multiplex detection and characterization of breast cancer exosomes by magneto-actuated immunoassay. *Talanta*. 2020;211:120657–120666. doi:10.1016/j.talanta.2019.120657
116. He F, Liu H, Guo X, Yin BC, Ye BC. Direct exosome quantification via bivalent-cholesterol-labeled DNA anchor for signal amplification. *Anal Chem*. 2017;89:12968–12975. doi:10.1021/acs.analchem.7b03919
117. Zeng R, Wang J, Wang Q, Tang D, Lin Y. Horseradish peroxidase-encapsulated DNA nanoflowers: an innovative signal-generation tag for colorimetric biosensor. *Talanta*. 2021;221:121600–121607. doi:10.1016/j.talanta.2020.121600
118. Yang Y, Li C, Shi H, Chen T, Wang Z, Li G. A pH-responsive bioassay for paper-based diagnosis of exosomes via mussel-inspired surface chemistry. *Talanta*. 2019;192:325–330. doi:10.1016/j.talanta.2018.09.067
119. Xu L, Chopdat R, Li D, Al-Jamal KT. Development of a simple, sensitive and selective colorimetric aptasensor for the detection of cancer-derived exosomes. *Biosens Bioelectron*. 2020;169:112576–112586. doi:10.1016/j.bios.2020.112576
120. Maiolo D, Paolini L, Di Noto G, et al. Colorimetric nanoplasmonic assay to determine purity and titrate extracellular vesicles. *Anal Chem*. 2015;87:4168–4176. doi:10.1021/ac504861d
121. Jiang Y, Shi M, Liu Y, et al. Aptamer/AuNP biosensor for colorimetric profiling of exosomal proteins. *Angew Chem*. 2017;129:12078–12082. doi:10.1002/ange.201703807
122. Liu W, Li J, Wu Y, Xing S, Lai Y, Zhang G. Target-induced proximity ligation triggers recombinase polymerase amplification and transcription-mediated amplification to detect tumor-derived exosomes in nasopharyngeal carcinoma with high sensitivity. *Biosens Bioelectron*. 2018;102:204–210. doi:10.1016/j.bios.2017.11.033
123. Lopez-Cobo S, Campos-Silva C, Moyano A, et al. Immunoassays for scarce tumour-antigens in exosomes: detection of the human NKG2D-ligand, MICA, in tetraspanin-containing nanovesicles from melanoma. *J Nanobiotechnol*. 2018;16:47–59. doi:10.1186/s12951-018-0372-z
124. Oliveira-Rodriguez M, Lopez-Cobo S, Reyburn HT, et al. Development of a rapid lateral flow immunoassay test for detection of exosomes previously enriched from cell culture medium and body fluids. *J Extracell Vesicles*. 2016;5:31803–31814. doi:10.3402/jev.v5.31803
125. Oliveira-Rodriguez M, Serrano-Pertierra E, Garcia AC, et al. Point-of-care detection of extracellular vesicles: sensitivity optimization and multiple-target detection. *Biosens Bioelectron*. 2017;87:38–45. doi:10.1016/j.bios.2016.08.001
126. Wu T, Yang Y, Cao Y, et al. Enhanced lateral flow assay with double conjugates for the detection of exosomes. *Sci China Chem*. 2018;61:1423–1429. doi:10.1007/s11426-018-9305-6
127. Zhang Y, Wang D, Yue S, et al. Sensitive multicolor visual detection of exosomes via dual signal amplification strategy of enzyme-catalyzed metallization of Au nanorods and hybridization chain reaction. *ACS Sens*. 2019;4:3210–3218. doi:10.1021/acssensors.9b01644
128. Zhang Y, Jiao J, Wei Y, Wang D, Yang C, Xu Z. Plasmonic colorimetric biosensor for sensitive exosome detection via enzyme-induced etching of gold nanobipyramid@MnO2 nanosheet nanostructures. *Anal Chem*. 2020;92:15244–15252. doi:10.1021/acs.analchem.0c04136
129. Farhana FZ, Umer M, Saeed A, et al. Isolation and detection of exosomes using Fe2O3 nanoparticles. *ACS Appl Nano Mater*. 2021;4:1175–1186. doi:10.1021/acsanm.0c02807

130. Liu B, Liu J. Accelerating peroxidase mimicking nanozymes using DNA. *Nanoscale*. 2015;7:13831–13835. doi:10.1039/C5NR04176G
131. Chen J, Xu Y, Lu Y, Xing W. Isolation and visible detection of tumor-derived exosomes from plasma. *Anal Chem*. 2018;90:14207–14215. doi:10.1021/acs.analchem.8b03031
132. Wang YM, Liu JW, Adkins GB, et al. Enhancement of the intrinsic peroxidase-like activity of graphitic carbon nitride nanosheets by ssDNAs and its application for detection of exosomes. *Anal Chem*. 2017;89:12327–12333. doi:10.1021/acs.analchem.7b03335
133. Xia Y, Liu M, Wang L, et al. A visible and colorimetric aptasensor based on DNA-capped single-walled carbon nanotubes for detection of exosomes. *Biosens Bioelectron*. 2017;92:8–15. doi:10.1016/j.bios.2017.01.063
134. Zhang Y, Su Q, Song D, Fan J, Xu Z. Label-free detection of exosomes based on ssDNA-modulated oxidase-mimicking activity of CuCo₂O₄ nanorods. *Anal Chim Acta*. 2021;1145:9–16. doi:10.1016/j.aca.2020.12.018
135. Shpacovitch V, Hergenroder R. Optical and surface plasmonic approaches to characterize extracellular vesicles. A review. *Anal Chim Acta*. 2018;1005:1–15. doi:10.1016/j.aca.2017.11.066
136. Jackman JA, Yorulmaz Avsar S, Ferhan AR, et al. Quantitative profiling of nanoscale liposome deformation by a localized surface plasmon resonance sensor. *Anal Chem*. 2017;89:1102–1109. doi:10.1021/acs.analchem.6b02532
137. Liu C, Zeng X, An Z, et al. Sensitive detection of exosomal proteins via a compact surface plasmon resonance biosensor for cancer diagnosis. *ACS Sens*. 2018;3:1471–1479. doi:10.1021/acssensors.8b00230
138. Picciolini S, Gualerzi A, Vanna R, et al. Detection and characterization of different brain-derived subpopulations of plasma exosomes by surface plasmon resonance imaging. *Anal Chem*. 2018;90:8873–8880. doi:10.1021/acs.analchem.8b00941
139. Rupert DL, Lasser C, Eldh M, et al. Determination of exosome concentration in solution using surface plasmon resonance spectroscopy. *Anal Chem*. 2014;86:5929–5936. doi:10.1021/ac500931f
140. Rupert DLM, Shelke GV, Emilsson G, et al. Dual-wavelength surface plasmon resonance for determining the size and concentration of sub-populations of extracellular vesicles. *Anal Chem*. 2016;88:9980–9988. doi:10.1021/acs.analchem.6b01860
141. Thakur A, Qiu G, Ng SP, et al. Direct detection of two different tumor-derived extracellular vesicles by SAM-AuNIs LSPR biosensor. *Biosens Bioelectron*. 2017;94:400–407. doi:10.1016/j.bios.2017.03.036
142. Yang Y, Zhai C, Zeng Q, Khan AL, Yu H. Multifunctional detection of extracellular vesicles with surface plasmon resonance microscopy. *Anal Chem*. 2020;92:4884–4890. doi:10.1021/acs.analchem.9b04622
143. Zhu L, Wang K, Cui J, et al. Label-free quantitative detection of tumor-derived exosomes through surface plasmon resonance imaging. *Anal Chem*. 2014;86:8857–8864. doi:10.1021/ac5023056
144. Im H, Shao H, Park YI, et al. Label-free detection and molecular profiling of exosomes with a nano-plasmonic sensor. *Nat Biotechnol*. 2014;32:490–495. doi:10.1038/nbt.2886
145. Mao Z, Zhao J, Chen J, Hu X, Koh K, Chen H. A simple and direct spr platform combining three-in-one multifunctional peptides for ultra-sensitive detection of PD-L1 exosomes. *Sens Actuat B Chem*. 2021;346:130496–130505. doi:10.1016/j.snb.2021.130496
146. Reiner AT, Ferrer NG, Venugopalan P, Lai RC, Lim SK, Dostalek J. Magnetic nanoparticle-enhanced surface plasmon resonance biosensor for extracellular vesicle analysis. *Analyst*. 2017;142:3913–3921. doi:10.1039/C7AN00469A
147. Di Noto G, Bugatti A, Zendrini A, et al. Merging colloidal nanoplasmonics and surface plasmon resonance spectroscopy for enhanced profiling of multiple myeloma-derived exosomes. *Biosens Bioelectron*. 2016;77:518–524. doi:10.1016/j.bios.2015.09.061
148. Fan Y, Duan X, Zhao M, et al. High-sensitive and multiplex biosensing assay of NSCLC-derived exosomes via different recognition sites based on SPRi array. *Biosens Bioelectron*. 2020;154:112066–112073. doi:10.1016/j.bios.2020.112066
149. Park J, Im H, Hong S, Castro CM, Weissleder R, Lee H. Analyses of intravesicular exosomal proteins using a nano-plasmonic system. *ACS Photonics*. 2018;5:487–494. doi:10.1021/acsp Photonics.7b00992
150. Wang C, Wang C, Jin D, et al. AuNP-amplified surface acoustic wave sensor for the quantification of exosomes. *ACS Sens*. 2020;5:362–369. doi:10.1021/acssensors.9b01869
151. Wang Q, Zou L, Yang X, et al. Direct quantification of cancerous exosomes via surface plasmon resonance with dual gold nanoparticle-assisted signal amplification. *Biosens Bioelectron*. 2019;135:129–136. doi:10.1016/j.bios.2019.04.013
152. Liao G, Liu X, Yang X, et al. Surface plasmon resonance assay for exosomes based on aptamer recognition and polydopamine-functionalized gold nanoparticles for signal amplification. *Microchim Acta*. 2020;187:251–260. doi:10.1007/s00604-020-4183-1
153. Chen W, Li J, Wei X, et al. Surface plasmon resonance biosensor using hydrogel-AuNP supramolecular spheres for determination of prostate cancer-derived exosomes. *Microchim Acta*. 2020;187:590–600. doi:10.1007/s00604-020-04573-4
154. Shin H, Oh S, Hong S, et al. Early-stage lung cancer diagnosis by deep learning-based spectroscopic analysis of circulating exosomes. *ACS Nano*. 2020;14:5435–5444. doi:10.1021/acsnano.9b09119
155. Avella-Oliver M, Puchades R, Wachsmann-Hogiu S, Maquieira A. Label-free SERS analysis of proteins and exosomes with large-scale substrates from recordable compact disks. *Sens Actuat B Chem*. 2017;252:657–662. doi:10.1016/j.snb.2017.06.058
156. Dong S, Wang Y, Liu Z, et al. Beehive-inspired macroporous SERS probe for cancer detection through capturing and analyzing exosomes in plasma. *ACS Appl Mater Interfaces*. 2020;12:5136–5146. doi:10.1021/acsami.9b21333
157. Lee W, Nanou A, Rikkert L, et al. Label-free prostate cancer detection by characterization of extracellular vesicles using Raman spectroscopy. *Anal Chem*. 2018;90:11290–11296. doi:10.1021/acs.analchem.8b01831
158. Park J, Hwang M, Choi B, et al. Exosome classification by pattern analysis of surface-enhanced Raman spectroscopy data for lung cancer diagnosis. *Anal Chem*. 2017;89:6695–6701. doi:10.1021/acs.analchem.7b00911
159. Yan Z, Dutta S, Liu Z, et al. A label-free platform for identification of exosomes from different sources. *ACS Sens*. 2019;4:488–497. doi:10.1021/acssensors.8b01564
160. Hou M, He D, Bu H, et al. A sandwich-type surface-enhanced Raman scattering sensor using dual aptamers and gold nanoparticles for the detection of tumor extracellular vesicles. *Analyst*. 2020;145:6232–6236. doi:10.1039/D0AN01385D
161. Li TD, Zhang R, Chen H, et al. An ultrasensitive polydopamine bi-functionalized SERS immunoassay for exosome-based diagnosis and classification of pancreatic cancer. *Chem Sci*. 2018;9:5372–5382. doi:10.1039/C8SC01611A
162. Tian YF, Ning CF, He F, Yin BC, Ye BC. Highly sensitive detection of exosomes by SERS using gold nanostar@Raman reporter@nanoshell structures modified with a bivalent cholesterol-labeled DNA anchor. *Analyst*. 2018;143:4915–4922. doi:10.1039/C8AN01041B

163. Zong S, Wang L, Chen C, et al. Facile detection of tumor-derived exosomes using magnetic nanobeads and SERS nanoprobe. *Anal Methods*. 2016;8:5001–5008. doi:10.1039/C6AY00406G
164. Zhang W, Jiang L, Diefenbach RJ, et al. Enabling sensitive phenotypic profiling of cancer-derived small extracellular vesicles using surface-enhanced Raman spectroscopy nanotags. *ACS Sens*. 2020;5:764–771. doi:10.1021/acssensors.9b02377
165. Di H, Zeng E, Zhang P, et al. General approach to engineering extracellular vesicles for biomedical analysis. *Anal Chem*. 2019;91:12752–12759. doi:10.1021/acs.analchem.9b02268
166. Wang Z, Zong S, Wang Y, et al. Screening and multiple detection of cancer exosomes using an SERS-based method. *Nanoscale*. 2018;10:9053–9062. doi:10.1039/C7NR09162A
167. Kwizera EA, O'Connor R, Vinduska V, et al. Molecular detection and analysis of exosomes using surface-enhanced Raman scattering gold nanorods and a miniaturized device. *Theranostics*. 2018;8:2722–2738. doi:10.7150/thno.21358
168. Ning CF, Wang L, Tian YF, Yin BC, Ye BC. Multiple and sensitive SERS detection of cancer-related exosomes based on gold-silver bimetallic nanotrepangs. *Analyst*. 2020;145:2795–2804. doi:10.1039/C9AN02180A
169. Zhang X, Liu C, Pei Y, Song W, Zhang S. Preparation of a novel Raman probe and its application in the detection of circulating tumor cells and exosomes. *ACS Appl Mater Interfaces*. 2019;11:28671–28680. doi:10.1021/acsami.9b09465
170. Dai Y, Bai S, Hu C, Chu K, Shen B, Smith ZJ. Combined morpho-chemical profiling of individual extracellular vesicles and functional nanoparticles without labels. *Anal Chem*. 2020;92:5585–5594. doi:10.1021/acs.analchem.0c00607
171. Bagheri Hashkavayi A, Cha BS, Lee ES, Kim S, Park KS. Advances in exosome analysis methods with an emphasis on electrochemistry. *Anal Chem*. 2020;92:12733–12740. doi:10.1021/acs.analchem.0c02745
172. Ma X. Recent progress in electrochemical detection of tumor-derived exosomes. *Int J Electrochem Sci*. 2020;15:7954–7967. doi:10.20964/2020.08.101
173. Chen A, Chatterjee S. Nanomaterials based electrochemical sensors for biomedical applications. *Chem Soc Rev*. 2013;42:5425–5438. doi:10.1039/c3cs35518g
174. Cavallaro S, Horak J, Hääg P, et al. Label-free surface protein profiling of extracellular vesicles by an electrokinetic sensor. *ACS Sens*. 2019;4:1399–1408. doi:10.1021/acssensors.9b00418
175. Kilic T, Valinhas ATDS, Wall I, Renaud P, Carrara S. Label-free detection of hypoxia-induced extracellular vesicle secretion from MCF-7 cells. *Sci Rep*. 2018;8:9402–9411. doi:10.1038/s41598-018-27203-9
176. Suthar J, Parsons ES, Hoogenboom BW, Williams GR, Guldin S. Acoustic immunosensing of exosomes using a quartz crystal microbalance with dissipation monitoring. *Anal Chem*. 2020;92:4082–4093. doi:10.1021/acs.analchem.9b05736
177. Yadav S, Boriachek K, Islam MN, et al. An electrochemical method for the detection of disease-specific exosomes. *ChemElectroChem*. 2017;4:967–971. doi:10.1002/celec.201600391
178. Wang S, Zhang L, Wan S, et al. Aptasensor with expanded nucleotide using DNA nanotetrahedra for electrochemical detection of cancerous exosomes. *ACS Nano*. 2017;11:3943–3949. doi:10.1021/acsnano.7b00373
179. Li Q, Tofaris GK, Davis JJ. Concentration-normalized electroanalytical assaying of exosomal markers. *Anal Chem*. 2017;89:3184–3190. doi:10.1021/acs.analchem.6b05037
180. Vaidyanathan R, Naghibosadat M, Rauf S, et al. Detecting exosomes specifically: a multiplexed device based on alternating current electrohydrodynamic induced nanoshearing. *Anal Chem*. 2014;86:11125–11132. doi:10.1021/ac502082b
181. Liu Q, Yue X, Li Y, et al. A novel electrochemical aptasensor for exosomes determination and release based on specific host-guest interactions between cucurbit [7]uril and ferrocene. *Talanta*. 2021;232:122451–122458. doi:10.1016/j.talanta.2021.122451
182. Sun Y, Jin H, Jiang X, Gui R. Assembly of black phosphorus nanosheets and MOF to form functional hybrid thin-film for precise protein capture, dual-signal and intrinsic self-calibration sensing of specific cancer-derived exosomes. *Anal Chem*. 2020;92:2866–2875. doi:10.1021/acs.analchem.9b05583
183. Ramadan S, Lobo R, Zhang Y, et al. Carbon-dot-enhanced graphene field-effect transistors for ultrasensitive detection of exosomes. *ACS Appl Mater Interfaces*. 2021;13:7854–7864. doi:10.1021/acsami.0c18293
184. Yu Y, Li YT, Jin D, et al. Electrical and label-free quantification of exosomes with a reduced graphene oxide field effect transistor biosensor. *Anal Chem*. 2019;91:10679–10686. doi:10.1021/acs.analchem.9b01950
185. Wang L, Zeng L, Wang Y, et al. Electrochemical aptasensor based on multidirectional hybridization chain reaction for detection of tumorous exosomes. *Sens Actuat B Chem*. 2021;332:129471–129480. doi:10.1016/j.snb.2021.129471
186. Doldán X, Fagúndez P, Cayota A, Laíz J, Tosar JP. Electrochemical sandwich immunosensor for determination of exosomes based on surface marker-mediated signal amplification. *Anal Chem*. 2016;88:10466–10473. doi:10.1021/acs.analchem.6b02421
187. An Y, Jin T, Zhu Y, Zhang F, He P. An ultrasensitive electrochemical aptasensor for the determination of tumor exosomes based on click chemistry. *Biosens Bioelectron*. 2019;142:11503–11510. doi:10.1016/j.bios.2019.111503
188. Huang R, He L, Xia Y, et al. A sensitive aptasensor based on a hemin/g-quadruplex-assisted signal amplification strategy for electrochemical detection of gastric cancer exosomes. *Small*. 2019;15:1900735–1900742. doi:10.1002/sml.201900735
189. Jiang J, Yu Y, Zhang H, Cai C. Electrochemical aptasensor for exosomal proteins profiling based on DNA nanotetrahedron coupled with enzymatic signal amplification. *Anal Chim Acta*. 2020;1130:1–9. doi:10.1016/j.aca.2020.07.012
190. Sun Z, Wang L, Wu S, et al. An electrochemical biosensor designed by using Zr-based metal-organic frameworks for the detection of glioblastoma-derived exosomes with practical application. *Anal Chem*. 2020;92:3819–3826. doi:10.1021/acs.analchem.9b05241
191. Gu C, Bai L, Pu L, Gai P, Li F. Highly sensitive and stable self-powered biosensing for exosomes based on dual metal-organic frameworks nanocarriers. *Biosens Bioelectron*. 2021;176:112907–112913. doi:10.1016/j.bios.2020.112907
192. Cao Y, Wang Y, Yu X, Jiang X, Li G, Zhao J. Identification of programmed death ligand-1 positive exosomes in breast cancer based on DNA amplification-responsive metal-organic frameworks. *Biosens Bioelectron*. 2020;166:112452–112460. doi:10.1016/j.bios.2020.112452
193. Wang M, Pan Y, Wu S, et al. Detection of colorectal cancer-derived exosomes based on covalent organic frameworks. *Biosens Bioelectron*. 2020;169:112638–112645. doi:10.1016/j.bios.2020.112638
194. Boriachek K, Masud MK, Palma C, et al. Avoiding pre-isolation step in exosome analysis: direct isolation and sensitive detection of exosomes using gold-loaded nanoporous ferric oxide nanozymes. *Anal Chem*. 2019;91:3827–3834. doi:10.1021/acs.analchem.8b03619
195. Zhang H, Wang Z, Wang F, Zhang Y, Wang H, Liu Y. Ti3C2 MXene mediated Prussian blue in situ hybridization and electrochemical signal amplification for the detection of exosomes. *Talanta*. 2021;224:121879–121886. doi:10.1016/j.talanta.2020.121879

196. Boriachek K, Islam MN, Gopalan V, Lam AK, Nguyen NT, Shiddiky MJA. Quantum dot-based sensitive detection of disease specific exosome in serum. *Analyst*. 2017;142:2211–2219. doi:10.1039/C7AN00672A
197. Zhou YG, Mohamadi RM, Poudineh M, et al. Interrogating circulating microsomes and exosomes using metal nanoparticles. *Small*. 2016;12:727–732. doi:10.1002/smll.201502365
198. Moura SL, Martin CG, Marti M, Pividori MI. Electrochemical immunosensing of nanovesicles as biomarkers for breast cancer. *Biosens Bioelectron*. 2020;150:111882–111889. doi:10.1016/j.bios.2019.111882
199. Wei F, Yang J, Wong DT. Detection of exosomal biomarker by electric field-induced release and measurement (EFIRM). *Biosens Bioelectron*. 2013;44:115–121. doi:10.1016/j.bios.2012.12.046
200. Jeong S, Park J, Pathania D, Castro CM, Weissleder R, Lee H. Integrated magneto-electrochemical sensor for exosome analysis. *ACS Nano*. 2016;10:1802–1809. doi:10.1021/acsnano.5b07584
201. Xu H, Liao C, Zuo P, Liu Z, Ye BC. Magnetic-based microfluidic device for on-chip isolation and detection of tumor-derived exosomes. *Anal Chem*. 2018;90:13451–13458. doi:10.1021/acs.analchem.8b03272
202. Cao Y, Li L, Han B, Wang Y, Dai Y, Zhao J. A catalytic molecule machine-driven biosensing method for amplified electrochemical detection of exosomes. *Biosens Bioelectron*. 2019;141:111397–111403. doi:10.1016/j.bios.2019.111397
203. Miao P, Tang Y. A multipedal DNA walker for amplified detection of tumor exosomes. *Chem Commun*. 2020;56:4982–4985. doi:10.1039/D0CC01817A
204. Guo Y, Cao Q, Feng Q. Catalytic hairpin assembly-triggered DNA walker for electrochemical sensing of tumor exosomes sensitized with Ag@C core-shell nanocomposites. *Anal Chim Acta*. 2020;1135:55–63. doi:10.1016/j.aca.2020.08.036
205. Dong H, Chen H, Jiang J, Zhang H, Cai C, Shen Q. Highly sensitive electrochemical detection of tumor exosomes based on aptamer recognition-induced multi-DNA release and cyclic enzymatic amplification. *Anal Chem*. 2018;90:4507–4513. doi:10.1021/acs.analchem.7b04863
206. Zhao L, Sun R, He P, Zhang X. Ultrasensitive detection of exosomes by target-triggered three-dimensional DNA walking machine and exonuclease III-assisted electrochemical ratiometric biosensing. *Anal Chem*. 2019;91:14773–14779. doi:10.1021/acs.analchem.9b04282
207. Yang L, Yin X, An B, Li F. Precise capture and direct quantification of tumor exosomes via a highly efficient dual-aptamer recognition-assisted ratiometric immobilization-free electrochemical strategy. *Anal Chem*. 2021;93:1709–1716. doi:10.1021/acs.analchem.0c04308
208. Li R, An Y, Jin T, Zhang F, He P. Detection of MUC1 protein on tumor cells and their derived exosomes for breast cancer surveillance with an electrochemiluminescence aptasensor. *J Electroanal Chem*. 2021;882:115011–115020. doi:10.1016/j.jelechem.2021.115011
209. Feng Q, Ma P, Cao QH, Guo YH, Xu JJ. An aptamer-binding DNA walking machine for sensitive electrochemiluminescence detection of tumor exosomes. *Chem Commun*. 2019;56:269–272. doi:10.1039/C9CC08051A
210. Qiao B, Guo Q, Jiang J, et al. An electrochemiluminescent aptasensor for amplified detection of exosomes from breast tumor cells (MCF-7 cells) based on G-quadruplex/hemin dnazymes. *Analyst*. 2019;144:3668–3675. doi:10.1039/C9AN00181F
211. Zhang Y, Wang F, Zhang H, Wang H, Liu Y. Multivalency interface and g-C₃N₄ coated liquid metal nanoprobe signal amplification for sensitive electrogenerated chemiluminescence detection of exosomes and their surface proteins. *Anal Chem*. 2019;91:12100–12107. doi:10.1021/acs.analchem.9b03427
212. Guo Y, Cao Q, Zhao C, Feng Q. Stimuli-responsive DNA microcapsules for homogeneous electrochemiluminescence sensing of tumor exosomes. *Sens Actuat B Chem*. 2021;329:129136–129142. doi:10.1016/j.snb.2020.129136
213. Zhang H, Wang Z, Zhang Q, Wang F, Liu Y. Ti₃C₂ MXenes nanosheets catalyzed highly efficient electrogenerated chemiluminescence biosensor for the detection of exosomes. *Biosens Bioelectron*. 2019;124–125:184–190. doi:10.1016/j.bios.2018.10.016
214. Fang D, Zhao D, Zhang S, Huang Y, Dai H, Lin Y. Black phosphorus quantum dots functionalized MXenes as the enhanced dual-mode probe for exosomes sensing. *Sens Actuat B Chem*. 2020;305:127544–127552. doi:10.1016/j.snb.2019.127544
215. Zhang H, Wang Z, Wang F, Zhang Y, Wang H, Liu Y. In situ formation of gold nanoparticles decorated Ti₃C₂ MXenes nanoprobe for highly sensitive electrogenerated chemiluminescence detection of exosomes and their surface proteins. *Anal Chem*. 2020;92:5546–5553. doi:10.1021/acs.analchem.0c00469
216. Liu X, Wang Q, Chen J, Chen X, Yang W. Ultrasensitive electrochemiluminescence biosensor for the detection of tumor exosomes based on peptide recognition and luminol-AuNPs@g-C₃N₄ nanoprobe signal amplification. *Talanta*. 2021;221:121379–121386. doi:10.1016/j.talanta.2020.121379
217. Pei Y, Ge Y, Zhang X, Li Y. Cathodic photoelectrochemical aptasensor based on NiO/BiOI/Au NP composite sensitized with cdse for determination of exosomes. *Microchim Acta*. 2021;188:51–61. doi:10.1007/s00604-021-04716-1
218. Roda A, Mirasoli M, Michelini E, et al. Progress in chemical luminescence-based biosensors: a critical review. *Biosens Bioelectron*. 2016;76:164–179. doi:10.1016/j.bios.2015.06.017
219. Jiang Q, Liu Y, Wang L, Adkins GB, Zhong W. Rapid enrichment and detection of extracellular vesicles enabled by cus-enclosed microgels. *Anal Chem*. 2019;91:15951–15958. doi:10.1021/acs.analchem.9b04485
220. Wang Y, Liu Z, Wang X, et al. Rapid and quantitative analysis of exosomes by a chemiluminescence immunoassay using superparamagnetic iron oxide particles. *J Biomed Nanotechnol*. 2019;15:1792–1800. doi:10.1166/jbn.2019.2809
221. Yang JS, Lee JC, Byeon SK, Rha KH, Moon MH. Size dependent lipidomic analysis of urinary exosomes from patients with prostate cancer by flow field-flow fractionation and nanoflow liquid chromatography-tandem mass spectrometry. *Anal Chem*. 2017;89:2488–2496. doi:10.1021/acs.analchem.6b04634
222. Zhang L, Wang H, Zhao G, et al. Anti-Tim4 grafting strongly hydrophilic metal-organic frameworks immunoaffinity flake for high-efficiency capture and separation of exosomes. *Anal Chem*. 2021;93:6534–6543. doi:10.1021/acs.analchem.1c00528
223. Chang M, Wang Q, Qin W, Shi X, Xu G. Rational synthesis of aptamer-functionalized polyethylenimine-modified magnetic graphene oxide composites for highly efficient enrichment and comprehensive metabolomics analysis of exosomes. *Anal Chem*. 2020;92:15497–15505. doi:10.1021/acs.analchem.0c03374
224. Zhang N, Sun N, Deng C. Rapid isolation and proteome analysis of urinary exosome based on double interactions of Fe₃O₄@TiO₂-DNA aptamer. *Talanta*. 2021;221:121571–121579. doi:10.1016/j.talanta.2020.121571
225. Brown BA, Zeng X, Todd AR, et al. Charge detection mass spectrometry measurements of exosomes and other extracellular particles enriched from bovine milk. *Anal Chem*. 2020;92:3285–3292. doi:10.1021/acs.analchem.9b05173
226. Fang X, Duan Y, Adkins GB, et al. Highly efficient exosome isolation and protein analysis by an integrated nanomaterial-based platform. *Anal Chem*. 2018;90:2787–2795. doi:10.1021/acs.analchem.7b04861

227. Wang Y, Zhang K, Huang X, Qiao L, Liu B. Mass spectrometry imaging of mass tag immunoassay enables the quantitative profiling of biomarkers from dozens of exosomes. *Anal Chem*. 2021;93:709–714. doi:10.1021/acs.analchem.0c03904
228. Zhang XW, Liu MX, He MQ, Chen S, Yu YL, Wang JH. Integral multielement signals by DNA-programmed UCNP-AuNP nano-satellite assemblies for ultrasensitive ICP-MS detection of exosomal proteins and cancer identification. *Anal Chem*. 2021;93:6437–6445. doi:10.1021/acs.analchem.1c00152

International Journal of Nanomedicine

Dovepress

Publish your work in this journal

The International Journal of Nanomedicine is an international, peer-reviewed journal focusing on the application of nanotechnology in diagnostics, therapeutics, and drug delivery systems throughout the biomedical field. This journal is indexed on PubMed Central, MedLine, CAS, SciSearch®, Current Contents®/Clinical Medicine,

Journal Citation Reports/Science Edition, EMBase, Scopus and the Elsevier Bibliographic databases. The manuscript management system is completely online and includes a very quick and fair peer-review system, which is all easy to use. Visit <http://www.dovepress.com/testimonials.php> to read real quotes from published authors.

Submit your manuscript here: <https://www.dovepress.com/international-journal-of-nanomedicine-journal>